


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV051120\
 Data File : VV015979.D
 Acq On : 11 May 2020 10:36
 Operator : SY/MD
 Sample : BFB54
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB54

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue May 12 01:07:44 2020

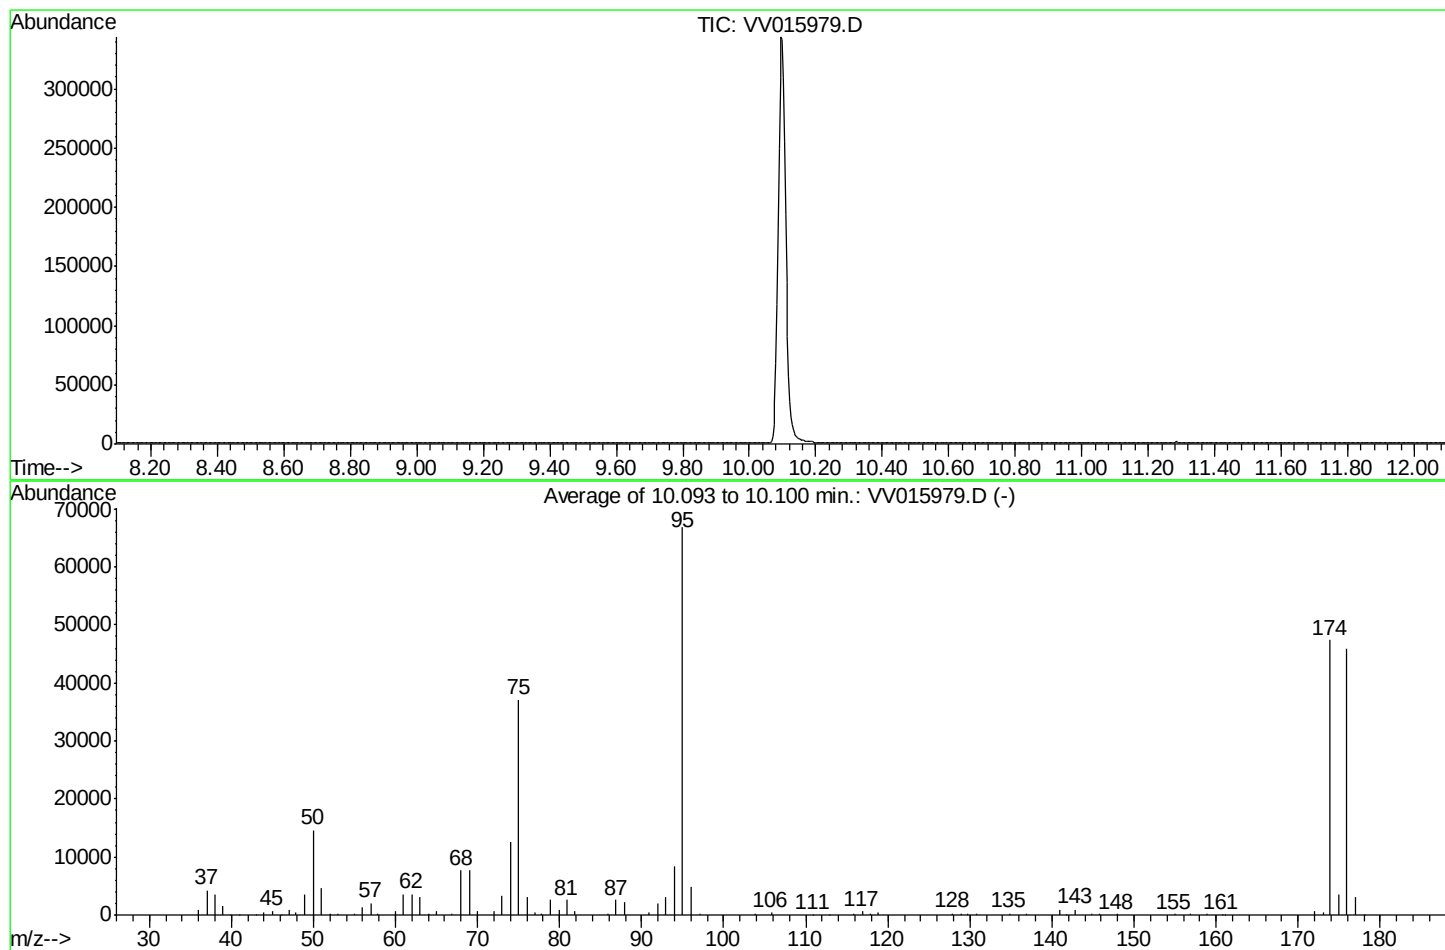

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	14570	PASS
75	95	30	80	55.6	37165	PASS
95	95	100	100	100.0	66816	PASS
96	95	5	9	7.2	4782	PASS
173	174	0.00	2	1.1	539	PASS
174	95	50	120	71.0	47418	PASS
175	174	5	9	7.7	3643	PASS
176	174	95	101	96.8	45885	PASS
177	176	5	9	6.8	3113	PASS

m/z	Abundance
36.00	863.0
37.00	4008.0
38.00	3500.0
39.00	1611.0
40.00	365.0
43.00	102.0
43.90	852.0
45.00	736.0
47.00	863.0
47.80	469.0
49.00	3260.0
50.00	13919.0
51.00	4398.0
52.00	287.0
52.90	136.0
55.00	218.0
56.00	1235.0
57.00	1971.0
57.90	168.0
59.90	582.0
61.00	3480.0
62.00	3310.0
63.00	2936.0
64.00	331.0
65.00	572.0
66.90	201.0
68.00	7369.0
69.00	7189.0
69.90	606.0
72.00	504.0
73.00	3037.0
74.00	11802.0
75.00	35184.0
76.00	3031.0
76.90	460.0
77.80	190.0
78.90	2560.0
79.90	772.0
80.90	2441.0
81.90	651.0
86.00	120.0
86.90	2581.0
87.90	2337.0
91.00	355.0
91.90	1783.0
92.90	2882.0
94.00	7788.0
95.00	62696.0
96.00	4517.0
97.00	126.0
103.80	358.0
105.90	374.0
115.80	301.0
116.90	547.0
117.80	255.0
118.80	401.0
127.90	304.0
128.90	152.0
129.80	269.0
130.90	115.0
134.80	217.0
136.90	165.0
140.90	764.0
142.90	841.0
144.80	159.0
145.70	123.0
147.90	160.0
154.90	151.0
156.80	106.0
158.90	117.0
160.70	143.0
172.00	706.0
173.10	738.0
173.90	43040.0
174.90	3376.0
175.90	41520.0
176.90	2788.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54

m/z	Abundance
36.00	986.0
37.00	4508.0
38.00	3754.0
39.00	1699.0
39.90	394.0
41.00	103.0
42.90	113.0
43.90	924.0
45.00	768.0
46.10	126.0
47.00	792.0
47.80	495.0
49.00	3662.0
50.00	15006.0
51.00	4820.0
52.00	257.0
52.90	143.0
55.00	260.0
56.00	1337.0
57.00	2078.0
57.80	179.0
60.00	635.0
61.00	3735.0
62.00	3802.0
63.00	3223.0
64.00	323.0
65.00	594.0
66.80	238.0
68.00	7938.0
69.00	7939.0
69.90	609.0
72.00	593.0
73.00	3303.0
74.00	13096.0
75.00	38560.0
76.00	3275.0
76.90	477.0
77.80	230.0
78.90	2834.0
79.90	884.0
80.90	2693.0
81.90	663.0
85.90	144.0
86.90	2726.0
87.90	2386.0
91.00	375.0
92.00	2054.0
93.00	3287.0
94.00	8579.0
95.00	69120.0
96.00	4976.0
97.00	144.0
103.90	345.0
105.80	390.0
110.90	105.0
112.80	102.0
115.80	311.0
116.90	663.0
117.80	261.0
118.80	460.0
127.90	340.0
128.90	162.0
129.70	309.0
130.80	141.0
134.80	258.0
137.00	159.0
140.90	889.0
141.80	120.0
142.80	955.0
144.80	152.0
145.80	142.0
147.90	157.0
154.90	174.0
156.80	121.0
158.80	121.0
160.80	107.0
161.00	109.0
171.90	769.0
173.10	881.0
173.90	49000.0
174.90	3705.0
175.90	47432.0
176.90	3192.0
178.10	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54

m/z	Abundance
36.00	879.0
37.00	4365.0
38.00	3596.0
39.00	1644.0
39.90	436.0
42.90	119.0
43.90	952.0
45.00	767.0
46.10	134.0
47.00	718.0
47.90	487.0
49.00	3598.0
50.00	14787.0
51.00	4589.0
52.00	227.0
52.90	144.0
55.00	272.0
56.00	1276.0
57.00	2050.0
57.80	164.0
60.00	618.0
61.00	3700.0
62.00	3822.0
63.00	3213.0
64.10	287.0
65.00	569.0
66.80	246.0
68.00	7810.0
69.00	7757.0
69.90	519.0
72.00	594.0
73.00	3297.0
74.00	13164.0
75.00	37752.0
76.00	3094.0
77.00	456.0
77.80	246.0
78.90	2741.0
79.90	913.0
80.90	2622.0
81.90	621.0
85.90	144.0
86.90	2553.0
87.90	2230.0
90.90	339.0
92.00	2147.0
93.00	3330.0
94.00	8607.0
95.00	68632.0
96.00	4854.0
97.10	147.0
103.80	306.0
105.90	371.0
110.90	102.0
112.90	104.0
115.80	252.0
116.90	702.0
117.80	260.0
118.80	439.0
127.90	345.0
128.90	148.0
129.80	306.0
130.80	164.0
134.80	214.0
137.00	134.0
140.90	889.0
141.80	140.0
142.80	984.0
144.90	141.0
145.80	142.0
147.90	142.0
155.00	193.0
156.80	133.0
158.80	124.0
171.90	722.0
173.90	50216.0
174.90	3850.0
175.90	48704.0
177.00	3359.0
178.00	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54

Scan 2788 (10.055 min): VV015979.D
BFB54

m/z	Abundance
39.90	342.0
44.00	439.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54