

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051123\
 Data File : VV031014.D
 Acq On : 11 May 2023 11:45
 Operator : SY/MD
 Sample : 02697-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031014.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	10	14	24	rVB2	9577	11588	2.10%	0.283%
2	1.281	68	75	89	rBV	76340	84591	15.33%	2.065%
3	1.535	147	154	165	rBV	72630	87417	15.84%	2.134%
4	2.063	309	318	337	rVB	166182	241784	43.83%	5.902%
5	2.458	432	441	450	rVB2	12684	22197	4.02%	0.542%
6	3.838	858	870	872	rBV	28188	48327	8.76%	1.180%
7	4.259	986	1001	1023	rBV	100729	257239	46.63%	6.279%
8	4.966	1204	1221	1244	rBV3	212833	551702	100.00%	13.467%
9	5.542	1387	1400	1421	rBV	133900	287437	52.10%	7.016%
10	5.998	1527	1542	1564	rBV	124807	270633	49.05%	6.606%
11	6.921	1818	1829	1842	rBV2	50935	97418	17.66%	2.378%
12	7.249	1917	1931	1956	rBV	235780	439893	79.73%	10.738%
13	7.564	2016	2029	2047	rBV	32184	64437	11.68%	1.573%
14	8.037	2166	2176	2217	rBV	159891	412480	74.76%	10.068%
15	8.792	2399	2411	2436	rBV	204173	361941	65.60%	8.835%
16	10.162	2824	2837	2850	rBV	86571	144421	26.18%	3.525%
17	10.336	2882	2891	2901	rVB3	6714	11731	2.13%	0.286%
18	11.194	3146	3158	3175	rBV	194843	324559	58.83%	7.922%
19	11.513	3247	3257	3261	rBV	4792	8218	1.49%	0.201%
20	11.567	3264	3274	3293	rVB	225615	362662	65.74%	8.852%
21	12.207	3468	3473	3483	rVB9	3991	6074	1.10%	0.148%




Sum of corrected areas: 4096749

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051123\
Data File : VV031014.D
Acq On : 11 May 2023 11:45
Operator : SY/MD
Sample : 02697-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

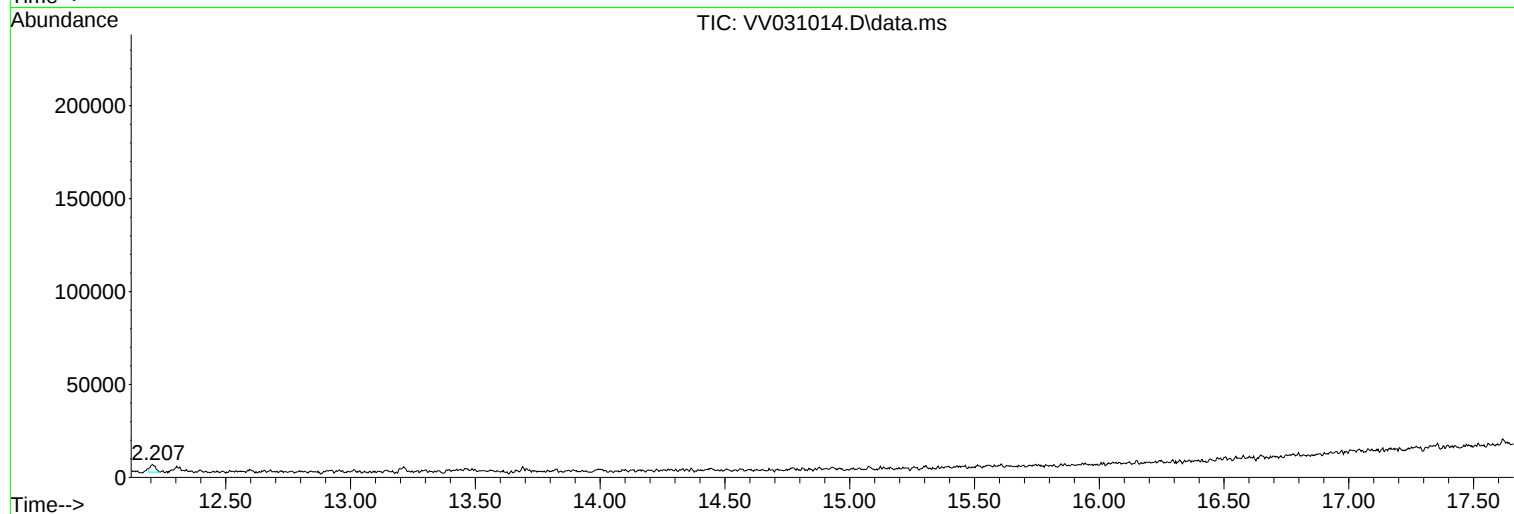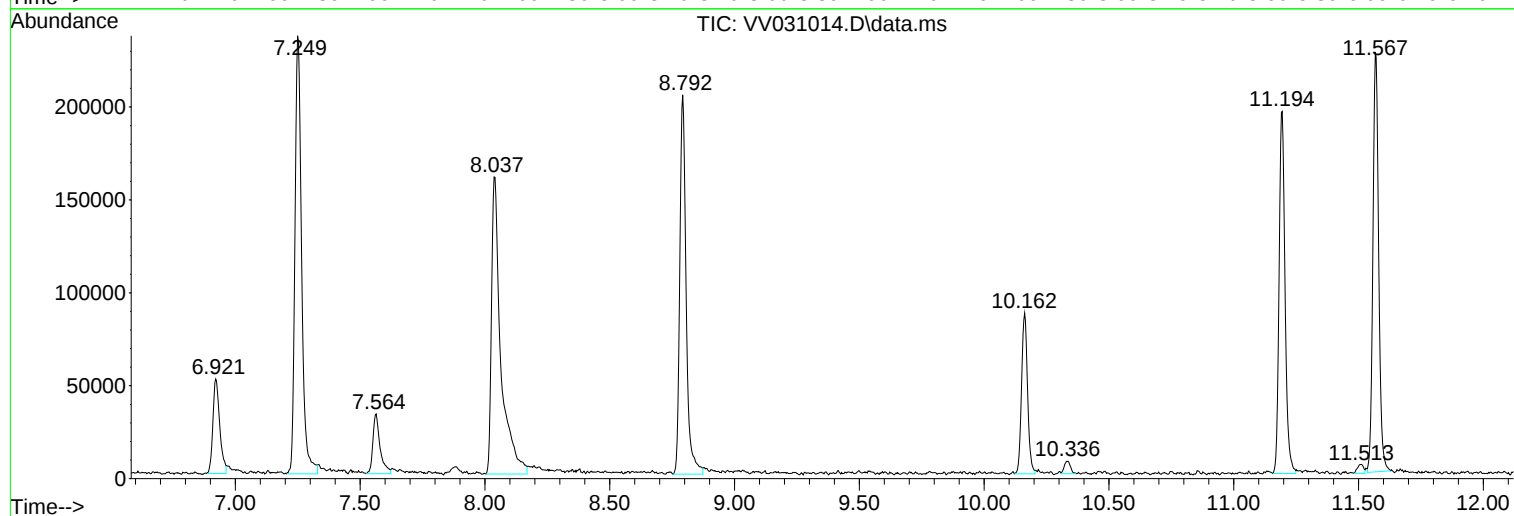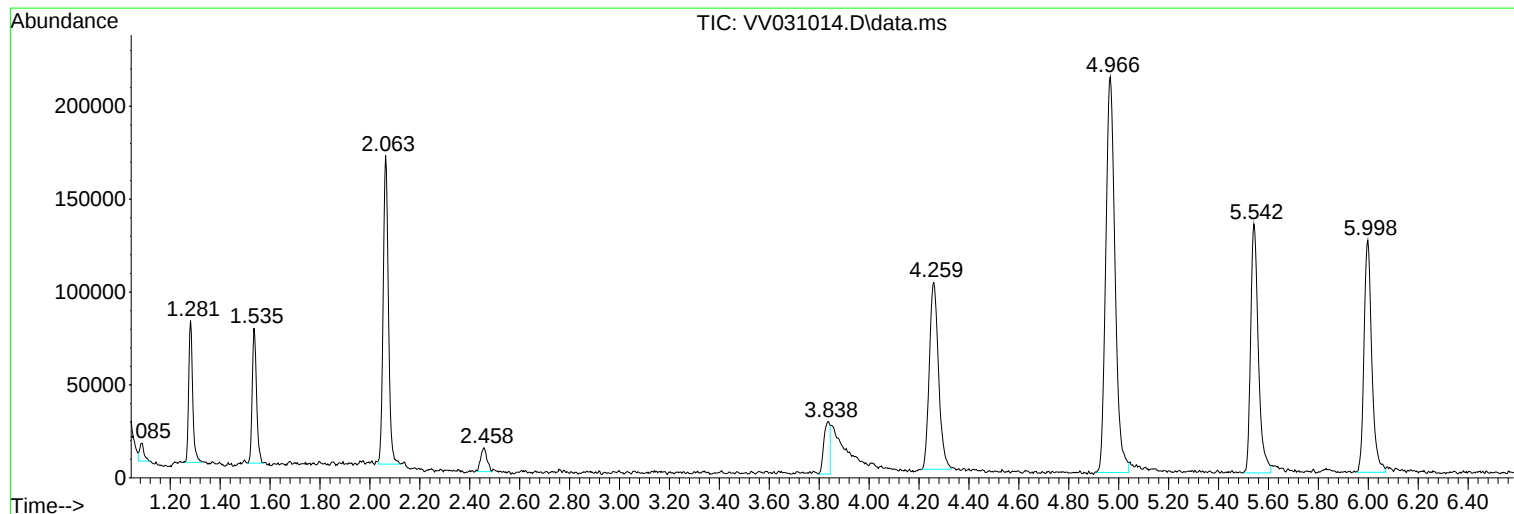

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051123\
Data File : VV031014.D
Acq On : 11 May 2023 11:45
Operator : SY/MD
Sample : 02697-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051123\
Data File : VV031014.D
Acq On : 11 May 2023 11:45
Operator : SY/MD
Sample : 02697-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc