
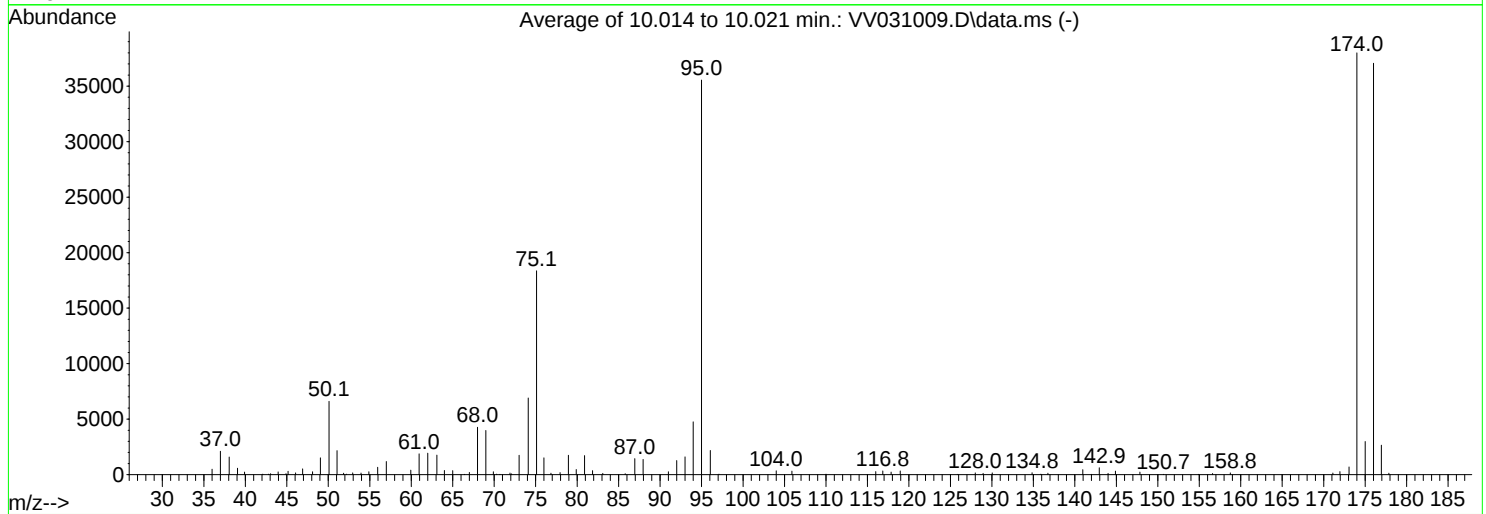


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051123\
 Data File : VV031009.D
 Acq On : 11 May 2023 09:03
 Operator : SY/MD
 Sample : BFB260
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB260

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat May 06 01:44:36 2023

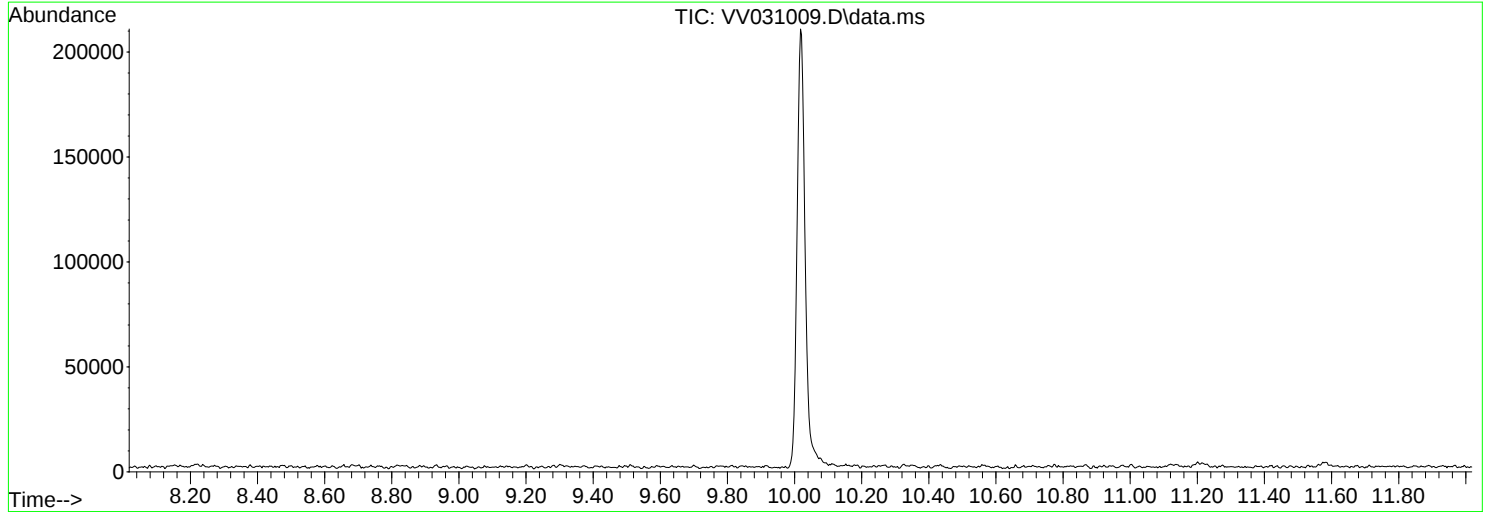

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	6605	PASS
75	95	30	80	51.6	18360	PASS
95	95	100	100	100.0	35547	PASS
96	95	5	9	6.1	2176	PASS
173	174	0.00	2	1.8	696	PASS
174	95	50	120	106.9	38000	PASS
175	174	5	9	7.9	2986	PASS
176	174	95	105	97.5	37061	PASS
177	176	5	10	7.1	2648	PASS

m/z	Abundance
35.70	200.0
37.80	168.0
38.60	150.0
39.10	128.0
40.20	167.0
41.20	142.0
43.90	225.0
46.50	102.0
58.10	116.0
60.80	104.0
74.30	122.0
77.40	108.0
83.40	105.0
94.60	115.0
104.90	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB260

m/z	Abundance
36.00	483.0
37.00	2040.0
38.00	1513.0
39.10	801.0
39.90	247.0
42.80	139.0
44.00	462.0
44.90	250.0
45.20	256.0
46.10	154.0
46.90	432.0
48.10	213.0
49.00	1507.0
50.10	6550.0
51.10	2037.0
51.80	116.0
52.90	154.0
53.90	156.0
54.90	247.0
56.00	631.0
57.00	1269.0
57.90	109.0
59.90	414.0
61.00	1878.0
62.00	1796.0
63.10	1766.0
64.00	409.0
65.00	297.0
67.00	205.0
68.00	4138.0
69.00	3746.0
69.80	239.0
70.30	114.0
71.90	241.0
73.00	1686.0
74.10	6772.0
75.10	17744.0
76.00	1427.0
76.80	150.0
78.00	220.0
78.90	1718.0
79.90	445.0
80.90	1651.0
81.80	371.0
83.10	125.0
87.00	1492.0
88.00	1365.0
91.00	214.0
92.00	1153.0
93.00	1661.0
94.00	4466.0
95.00	33816.0
96.10	2258.0
104.00	310.0
105.00	100.0
105.90	300.0
116.00	220.0
116.90	340.0
117.80	206.0
118.90	297.0
128.10	137.0
128.90	148.0
130.00	151.0
134.80	190.0
136.70	120.0
140.90	453.0
143.00	615.0
143.90	102.0
144.90	316.0
147.80	199.0
150.70	108.0
156.60	103.0
158.80	154.0
171.10	122.0
172.00	266.0
173.00	589.0
174.00	35648.0
175.00	2795.0
176.00	34648.0
176.90	2417.0
177.80	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB260

m/z	Abundance
36.00	514.0
37.00	2215.0
38.10	1637.0
39.10	681.0
39.90	229.0
43.00	128.0
44.00	458.0
45.20	319.0
46.10	161.0
46.90	541.0
48.10	277.0
49.10	1521.0
50.10	6810.0
51.10	2289.0
51.90	131.0
52.90	162.0
53.90	147.0
54.90	295.0
55.90	661.0
57.00	1256.0
57.90	109.0
59.90	408.0
61.00	2012.0
62.00	1979.0
63.10	1847.0
64.00	379.0
65.00	355.0
67.00	214.0
68.00	4433.0
69.00	4106.0
69.90	262.0
71.90	202.0
73.00	1848.0
74.10	7296.0
75.10	18776.0
76.00	1535.0
78.00	194.0
78.90	1765.0
79.90	474.0
80.90	1771.0
81.90	360.0
83.10	131.0
85.80	103.0
87.00	1477.0
88.00	1422.0
91.00	280.0
92.00	1303.0
93.00	1619.0
94.00	4860.0
95.00	36728.0
96.10	2207.0
104.00	369.0
105.00	105.0
105.90	355.0
116.00	293.0
116.90	336.0
117.80	250.0
119.00	328.0
128.00	165.0
128.90	101.0
130.10	165.0
134.80	191.0
136.70	131.0
140.90	465.0
142.00	107.0
143.00	643.0
144.00	126.0
144.90	325.0
147.80	239.0
156.60	103.0
158.80	174.0
171.10	155.0
172.00	284.0
173.10	736.0
174.00	39416.0
175.00	3112.0
176.00	38448.0
177.00	2811.0
177.90	133.0

Instrument :
MSVOA_V
ClientSampleId :
BFB260

m/z	Abundance
36.00	463.0
37.00	2083.0
38.10	1602.0
39.00	632.0
39.90	227.0
40.40	131.0
41.00	113.0
42.10	125.0
43.10	141.0
44.00	501.0
45.10	330.0
46.00	140.0
46.90	600.0
48.10	311.0
49.00	1511.0
50.10	6455.0
51.00	2165.0
51.90	141.0
52.20	124.0
53.00	173.0
54.00	151.0
54.90	257.0
55.90	686.0
57.00	1040.0
60.00	400.0
61.00	2060.0
62.00	2004.0
63.10	1642.0
64.00	342.0
65.00	417.0
66.40	110.0
67.00	178.0
68.00	4217.0
69.00	4084.0
70.00	262.0
70.70	109.0
72.10	197.0
73.00	1716.0
74.10	7037.0
75.10	18560.0
76.00	1579.0
76.90	222.0
77.90	169.0
79.00	1761.0
79.90	469.0
80.90	1719.0
81.90	360.0
83.10	109.0
85.80	142.0
86.90	1346.0
87.90	1314.0
91.00	283.0
92.00	1356.0
93.00	1533.0
94.00	4955.0
95.00	36096.0
96.00	2064.0
97.10	121.0
104.00	342.0
105.90	292.0
110.00	114.0
116.00	314.0
116.80	323.0
117.90	234.0
118.90	366.0
125.90	100.0
127.90	185.0
129.00	101.0
130.10	170.0
134.90	128.0
135.90	123.0
136.80	134.0
141.00	436.0
142.90	602.0
144.10	126.0
144.90	298.0
147.90	254.0
154.90	110.0
156.60	110.0
158.70	158.0
171.10	161.0
171.90	264.0
173.10	763.0
174.00	38936.0
175.00	3050.0
176.00	38088.0
177.00	2715.0
177.90	146.0

Instrument :
MSVOA_V
ClientSampleId :
BFB260