

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV051220\
 Data File : VV016010.D
 Acq On : 12 May 2020 13:32
 Operator : SY/MD
 Sample : L2598-01
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H41X3

Quant Time: May 13 07:27:12 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed May 13 06:55:36 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	143275	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	140831	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	65227	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	51780	6.66	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	133.20%#
7) Chloroethane-d5	1.58	69	47311	6.42	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	128.40%
11) 1,1-Dichloroethene-d2	2.12	63	78236	4.68	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	93.60%
20) 2-Butanone-d5	3.93	46	126183	56.91	ug/L	-0.04
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.82%
24) Chloroform-d	4.38	84	97307	5.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	114.60%
26) 1,2-Dichloroethane-d4	5.06	65	56417	5.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	115.80%
32) Benzene-d6	5.08	84	193474	5.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	115.40%
36) 1,2-Dichloropropane-d6	6.10	67	60398	5.91	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	118.20%
41) Toluene-d8	7.34	98	174887	5.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.40%
45) trans-1,3-Dichloropropene-	7.65	79	19784	4.93	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	98.60%
48) 2-Hexanone-d5	8.12	63	87232	49.46	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.92%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	37630	5.23	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.60%
65) 1,2-Dichlorobenzene-d4	11.65	152	62231	5.88	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	117.60%


Target Compounds					Ovalue
13) Acetone	2.21	43	5671	3.877 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV051220\
Data File : VV016010.D
Acq On : 12 May 2020 13:32
Operator : SY/MD
Sample : L2598-01
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H41X3

Quant Time: May 13 07:27:12 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed May 13 06:55:36 2020
Response via : Initial Calibration

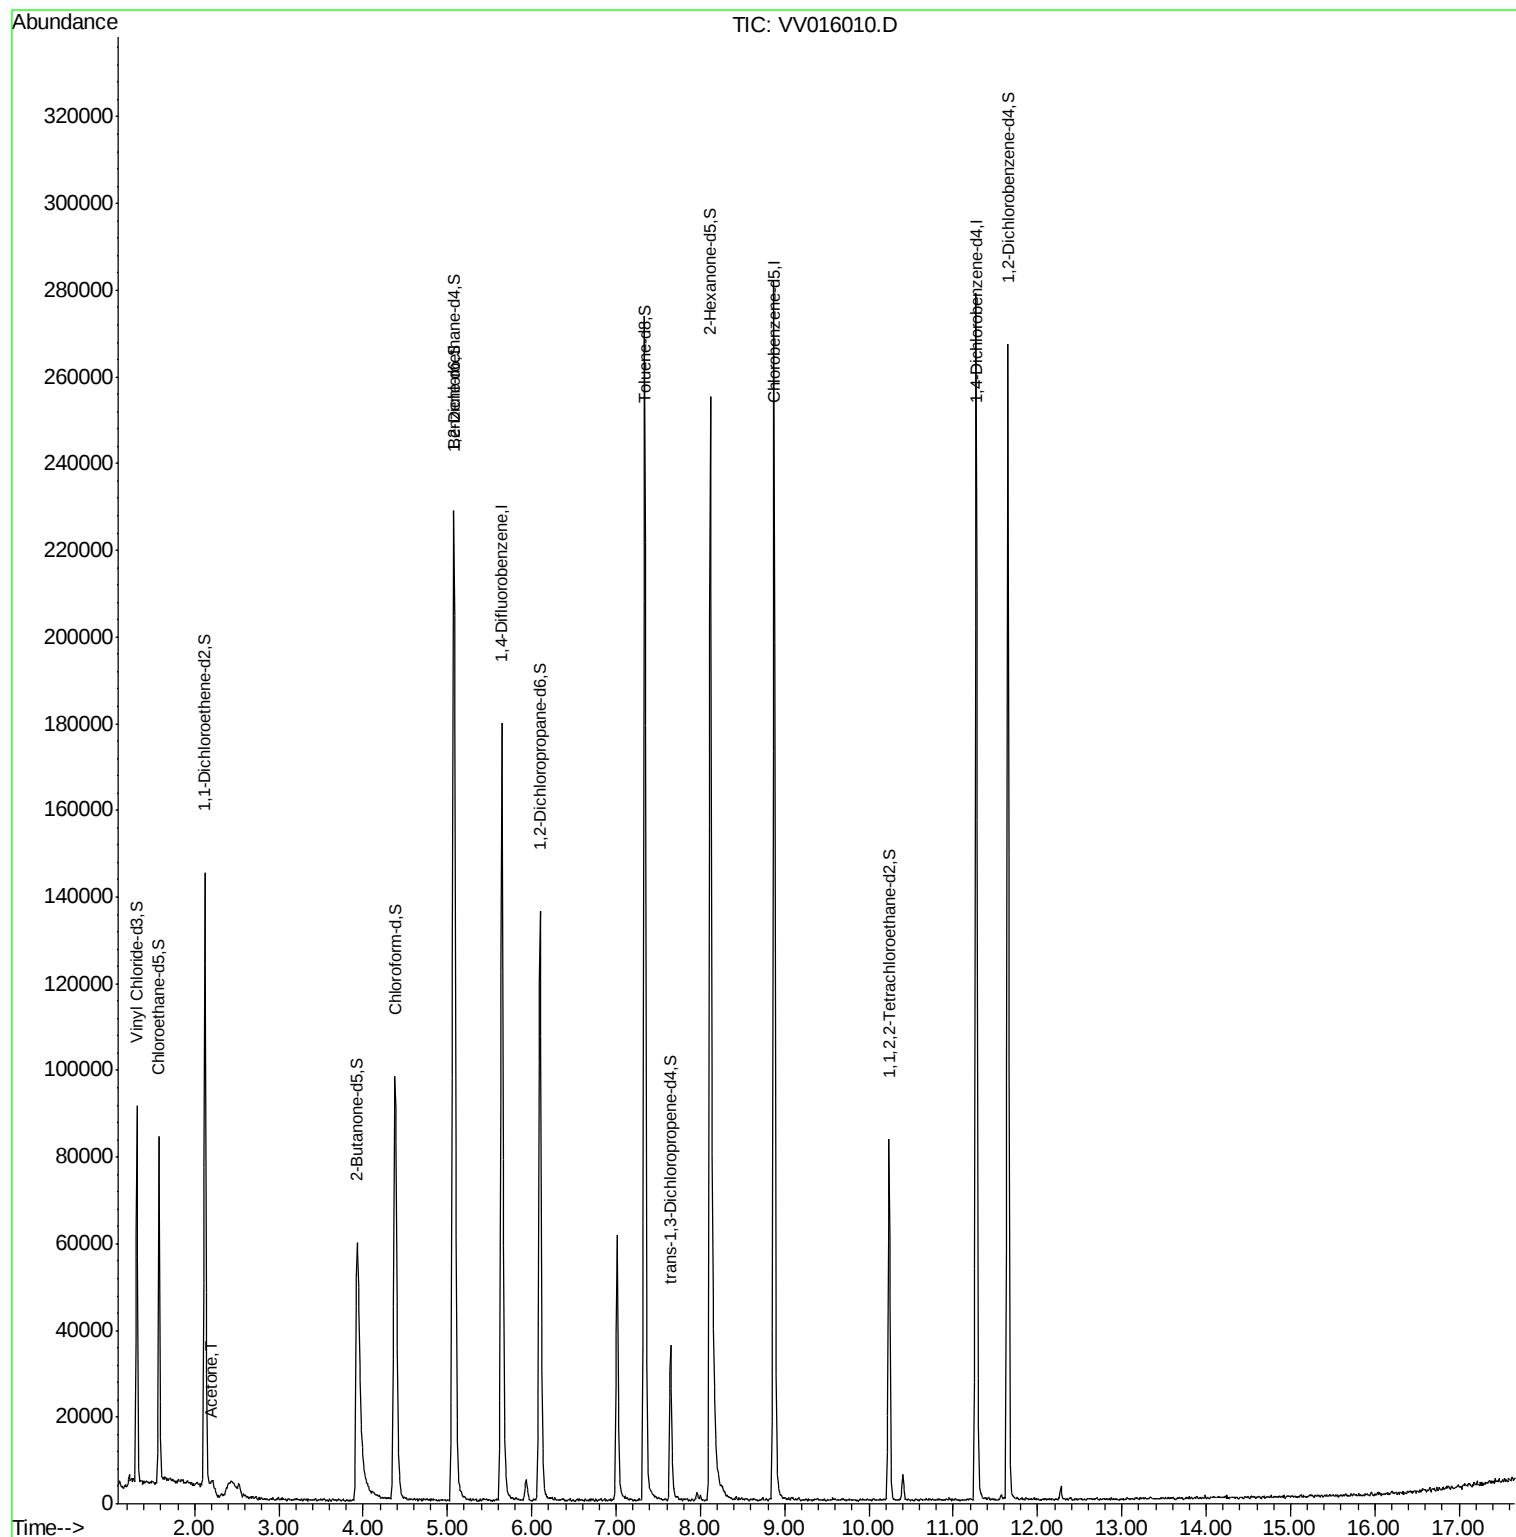

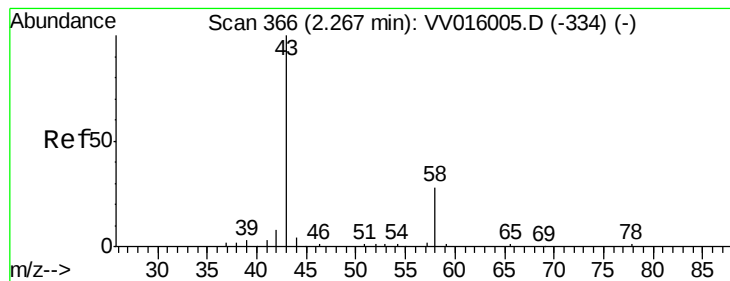

#13

Acetone

Concen: 3.877 ug/L

RT: 2.21 min Scan# 347

Delta R.T. -0.06 min

Lab File: VV016010.D

Acq: 12 May 2020 13:32

Instrument :

MSVOA_V

ClientSampleId :

H41X3

Tot Ion: 43 Resp: 5671

Ion Ratio Lower Upper

43 100

58 16.6 0.0 30.8

