

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV051220\
 Data File : VV016022.D
 Acq On : 12 May 2020 18:35
 Operator : SY/MD
 Sample : L2542-03
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4208

Quant Time: May 13 08:27:22 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed May 13 06:55:36 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	139461	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	138968	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	64535	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	27788	3.67	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	73.40%
7) Chloroethane-d5	1.58	69	29259	4.08	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.60%
11) 1,1-Dichloroethene-d2	2.12	63	48060	2.95	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.00%#
20) 2-Butanone-d5	3.94	46	115593	53.56	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.12%
24) Chloroform-d	4.38	84	77740	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.00%
26) 1,2-Dichloroethane-d4	5.06	65	44522	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.00%
32) Benzene-d6	5.08	84	145405	4.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.00%
36) 1,2-Dichloropropane-d6	6.10	67	47475	4.70	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.00%
41) Toluene-d8	7.34	98	129701	4.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.00%
45) trans-1,3-Dichloropropene-	7.65	79	15440	3.90	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.00%
48) 2-Hexanone-d5	8.12	63	76255	43.82	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.64%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	35827	5.05	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.00%
65) 1,2-Dichlorobenzene-d4	11.65	152	50221	4.79	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.80%


Target Compounds					Ovalue
13) Acetone	2.23	43	4436	3.116 ug/L #	49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV051220\
Data File : VV016022.D
Acq On : 12 May 2020 18:35
Operator : SY/MD
Sample : L2542-03
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4208

Quant Time: May 13 08:27:22 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed May 13 06:55:36 2020
Response via : Initial Calibration

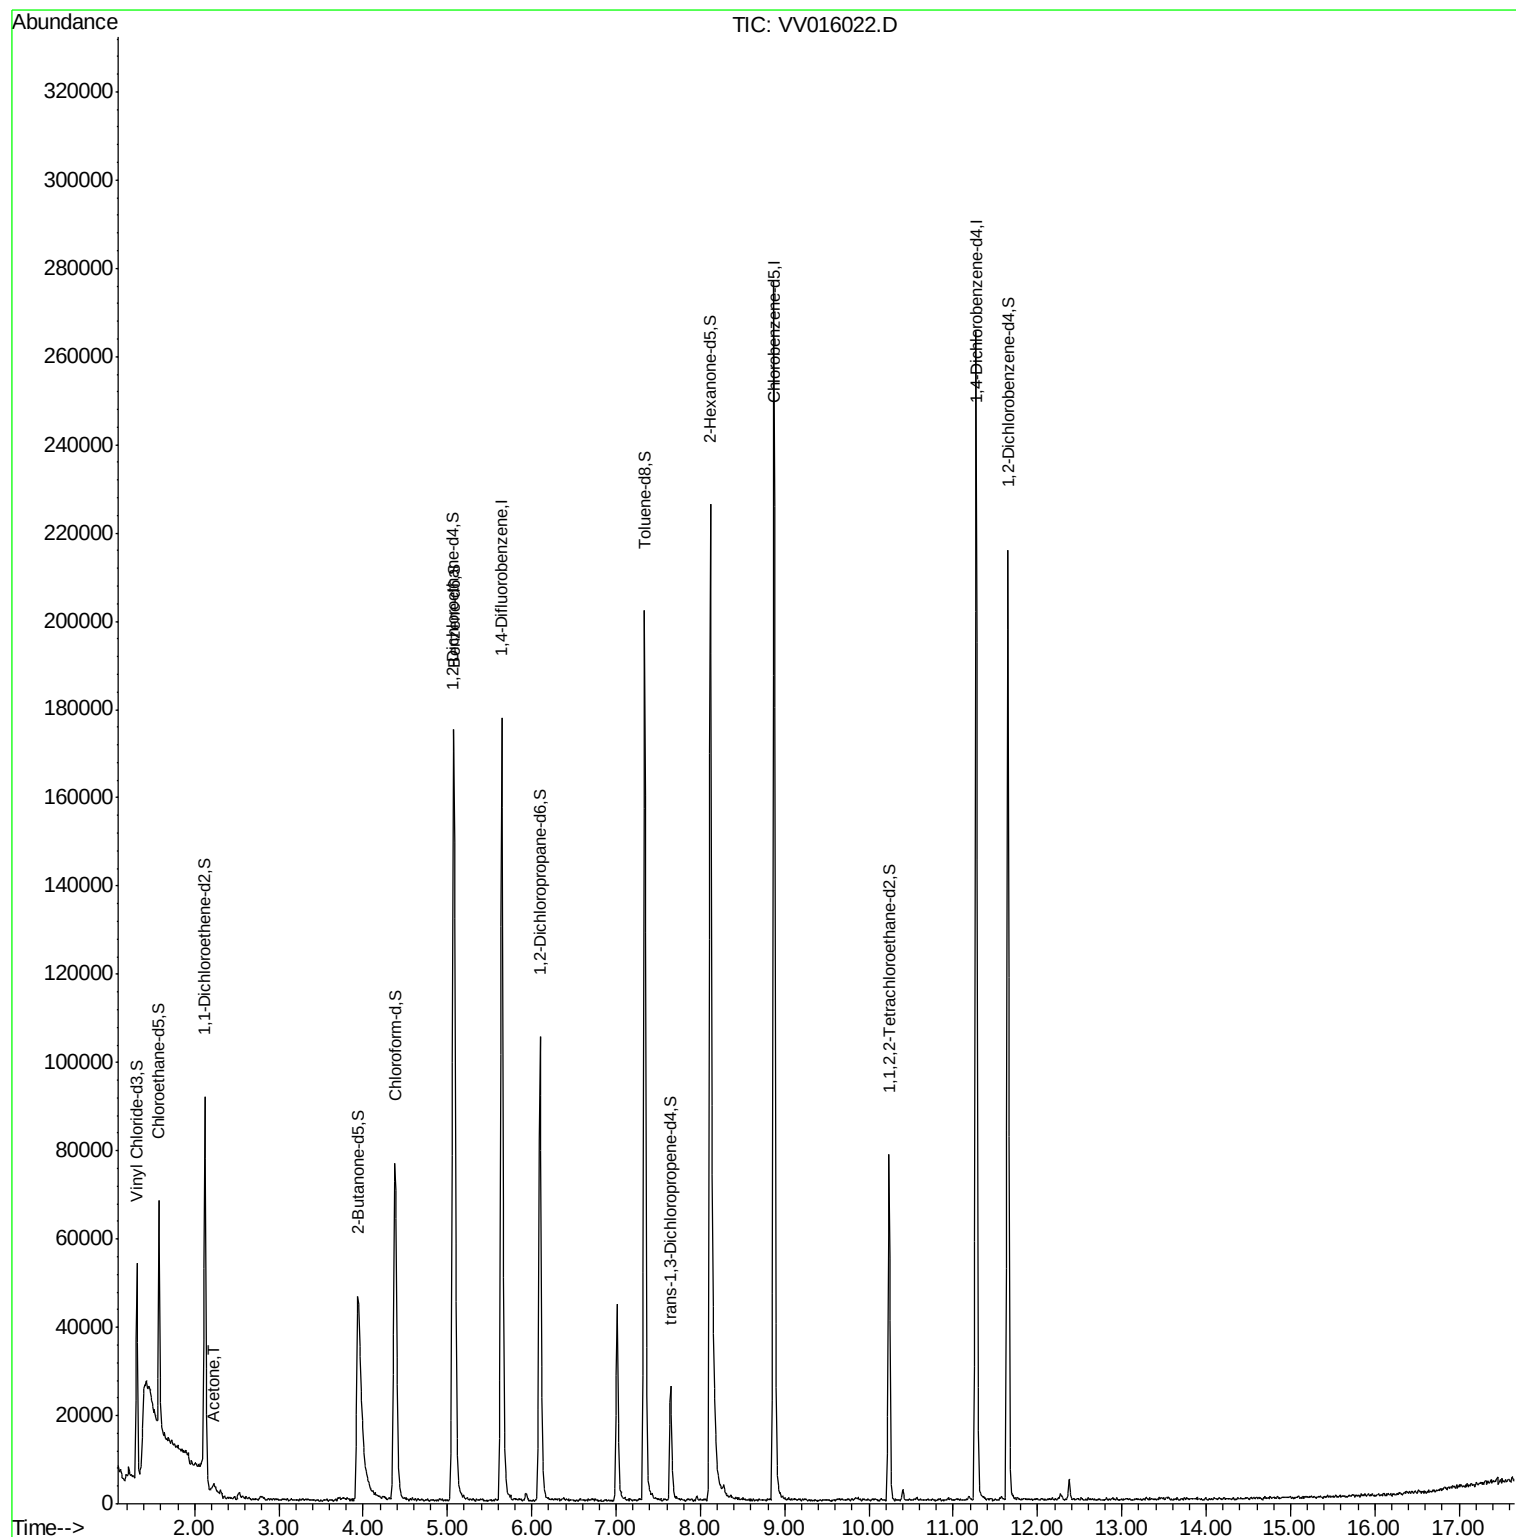

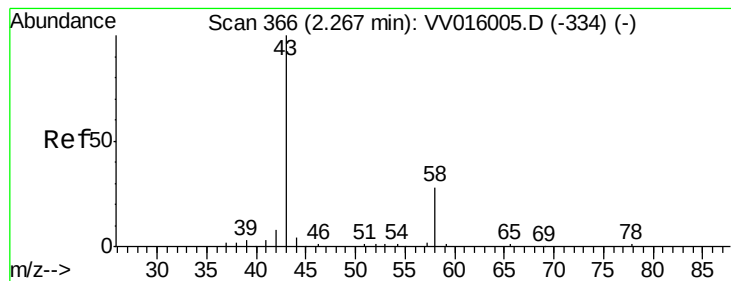

#13
 Acetone
 Concen: 3.116 ug/L
 RT: 2.23 min Scan# 355
 Delta R.T. -0.04 min
 Lab File: VV016022.D
 Acq: 12 May 2020 18:35

Instrument :
 MSVOA_V
 ClientSampleId :
 H4208

Tot Ion: 43 Resp: 4436
 Ion Ratio Lower Upper
 43 100
 58 36.9 0.0 30.8#

