


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV051220\
 Data File : VV016004.D
 Acq On : 12 May 2020 10:09
 Operator : SY/MD
 Sample : BFB55
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB55

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed May 13 06:55:36 2020

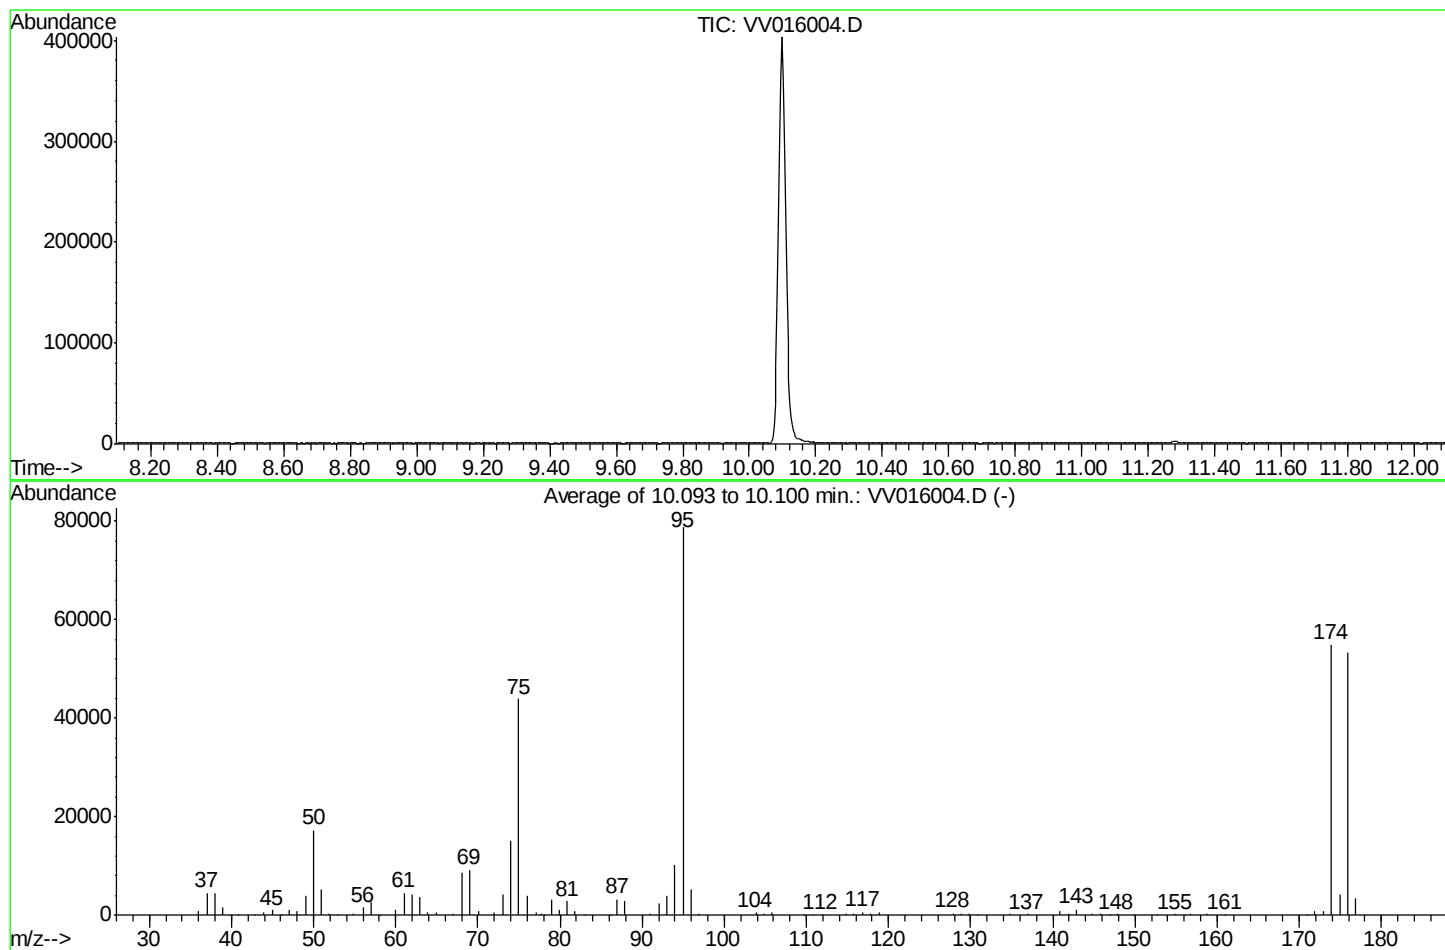

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	17239	PASS
75	95	30	80	55.7	43909	PASS
95	95	100	100	100.0	78770	PASS
96	95	5	9	6.7	5261	PASS
173	174	0.00	2	1.4	785	PASS
174	95	50	120	69.8	54989	PASS
175	174	5	9	7.8	4291	PASS
176	174	95	101	97.0	53346	PASS
177	176	5	9	6.5	3457	PASS

m/z	Abundance
36.00	856.0
37.00	4402.0
38.00	4194.0
39.00	1720.0
40.00	470.0
42.80	117.0
43.90	1034.0
45.00	926.0
47.00	983.0
48.00	658.0
49.00	3632.0
50.00	16069.0
51.00	4904.0
51.90	334.0
52.90	128.0
54.90	279.0
56.00	1506.0
57.00	2424.0
58.10	114.0
59.90	951.0
61.00	4226.0
62.00	3955.0
63.00	3434.0
63.90	419.0
65.00	449.0
67.00	230.0
68.00	8270.0
69.00	8627.0
70.10	798.0
72.00	556.0
73.00	3836.0
74.00	14217.0
75.00	41256.0
76.00	3750.0
77.10	553.0
77.80	343.0
78.90	2976.0
79.90	958.0
80.90	2853.0
81.80	744.0
82.90	107.0
87.00	2971.0
87.90	2555.0
90.90	266.0
92.00	2237.0
93.00	3600.0
94.00	9643.0
95.00	73752.0
96.00	5071.0
97.10	166.0
103.90	427.0
104.90	104.0
105.90	448.0
110.80	105.0
111.80	135.0
114.80	138.0
115.80	378.0
116.90	478.0
117.80	373.0
118.90	409.0
127.90	288.0
128.90	186.0
129.80	299.0
134.80	155.0
136.90	126.0
140.90	789.0
142.00	154.0
142.90	1047.0
144.80	193.0
145.80	143.0
147.80	245.0
152.70	101.0
154.90	182.0
156.70	147.0
158.80	149.0
160.90	102.0
170.80	106.0
171.90	721.0
173.00	742.0
173.90	50352.0
174.90	3918.0
175.90	48344.0
176.90	3289.0
177.90	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55

m/z	Abundance
36.00	909.0
37.00	4605.0
38.00	4469.0
39.00	1703.0
39.90	464.0
42.90	116.0
43.90	1085.0
45.00	995.0
46.10	113.0
47.00	1064.0
47.90	711.0
49.00	3956.0
50.00	17944.0
51.00	5321.0
51.90	323.0
53.00	144.0
54.90	332.0
56.00	1552.0
57.00	2642.0
58.10	109.0
59.90	1039.0
61.00	4600.0
62.00	4437.0
63.00	3888.0
63.90	454.0
65.00	588.0
67.00	258.0
68.00	9015.0
69.00	9507.0
70.10	833.0
72.00	608.0
73.00	4270.0
74.00	15636.0
75.00	45712.0
76.00	4180.0
77.00	655.0
77.80	366.0
78.90	3176.0
79.90	1107.0
80.90	2934.0
81.80	860.0
83.00	109.0
86.90	3377.0
87.90	2918.0
90.90	302.0
92.00	2320.0
93.00	4020.0
94.00	10558.0
95.00	81648.0
96.00	5460.0
96.90	178.0
103.90	487.0
104.80	143.0
105.90	467.0
114.80	180.0
115.80	358.0
116.90	579.0
117.80	391.0
118.90	468.0
127.90	337.0
128.90	170.0
129.80	313.0
130.80	105.0
134.70	164.0
136.90	173.0
140.90	825.0
141.90	150.0
142.90	1167.0
144.80	174.0
145.90	168.0
147.80	266.0
149.90	126.0
152.70	125.0
154.90	216.0
156.10	102.0
156.80	178.0
158.80	148.0
161.00	105.0
170.90	118.0
171.90	782.0
172.90	806.0
173.90	57048.0
174.90	4460.0
175.90	54944.0
176.90	3566.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55

m/z	Abundance
36.00	813.0
37.00	4425.0
38.00	4245.0
39.00	1641.0
39.90	413.0
40.80	101.0
42.90	108.0
44.00	1020.0
45.00	910.0
47.00	1040.0
47.90	620.0
49.00	3899.0
50.00	17704.0
51.00	5243.0
51.90	296.0
53.00	138.0
54.90	337.0
56.00	1500.0
57.00	2499.0
58.20	117.0
59.90	1026.0
61.00	4514.0
62.00	4500.0
63.00	3965.0
63.90	461.0
65.00	668.0
66.90	252.0
68.00	8813.0
69.00	9471.0
70.00	738.0
72.00	549.0
73.00	4269.0
74.00	15327.0
75.00	44760.0
76.00	4050.0
77.00	641.0
78.00	318.0
78.90	3032.0
79.90	1149.0
80.90	2742.0
81.90	857.0
83.00	108.0
86.10	127.0
86.90	3330.0
87.90	3006.0
90.90	305.0
92.00	2182.0
93.00	3987.0
94.00	10174.0
95.00	80912.0
96.00	5252.0
96.90	171.0
103.90	518.0
104.80	185.0
105.80	422.0
109.60	109.0
114.90	181.0
115.80	360.0
116.90	652.0
117.80	339.0
118.90	498.0
127.90	367.0
128.90	148.0
129.80	336.0
130.80	154.0
134.70	171.0
136.90	212.0
140.90	775.0
141.90	161.0
142.90	1134.0
144.70	156.0
145.90	151.0
146.90	102.0
147.90	254.0
149.90	114.0
154.90	216.0
156.00	126.0
156.80	174.0
158.80	133.0
170.90	114.0
171.90	754.0
172.90	808.0
173.90	57568.0
174.90	4497.0
175.90	56752.0
176.90	3517.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55

Scan 2788 (10.055 min): VV016004.D
BFB55

m/z	Abundance
39.90	337.0
44.00	416.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55