

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW051222\
 Data File : VW025879.D
 Acq On : 12 May 2022 13:55
 Operator : SY/MD
 Sample : N2746-06ME
 Misc : 5.56g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBSL2ME

Quant Time: May 13 07:08:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 13 07:07:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	336968	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	339098	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	155183	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	150953	34.711	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	69.420%
7) Chloroethane-d5	1.568	69	127308	33.334	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	66.660%#
11) 1,1-Dichloroethene-d2	2.108	63	227482	29.908	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	59.820%#
21) 2-Butanone-d5	3.902	46	130585	70.057	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	70.060%
24) Chloroform-d	4.342	84	233060	38.368	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	76.740%
26) 1,2-Dichloroethane-d4	5.027	65	150557	41.012	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.020%
32) Benzene-d6	5.043	84	469873	39.747	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	79.500%
36) 1,2-Dichloropropane-d6	6.066	67	152215	41.923	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	83.840%
41) Toluene-d8	7.313	98	401299	36.844	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	73.680%#
43) trans-1,3-Dichloroprop...	7.619	79	61814	38.138	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	76.280%
47) 2-Hexanone-d5	8.088	63	101455	76.216	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	76.220%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	191031	39.453	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	78.900%
66) 1,2-Dichlorobenzene-d4	11.622	152	152161	44.700	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.400%
Target Compounds						
61) 1,2,3-Trichloropropane	11.246	75	19460	6.335	ug/L	Qvalue # 65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
Data File : VV025879.D
Acq On : 12 May 2022 13:55
Operator : SY/MD
Sample : N2746-06ME
Misc : 5.56g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBSL2ME

Quant Time: May 13 07:08:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 13 07:07:32 2022
Response via : Initial Calibration

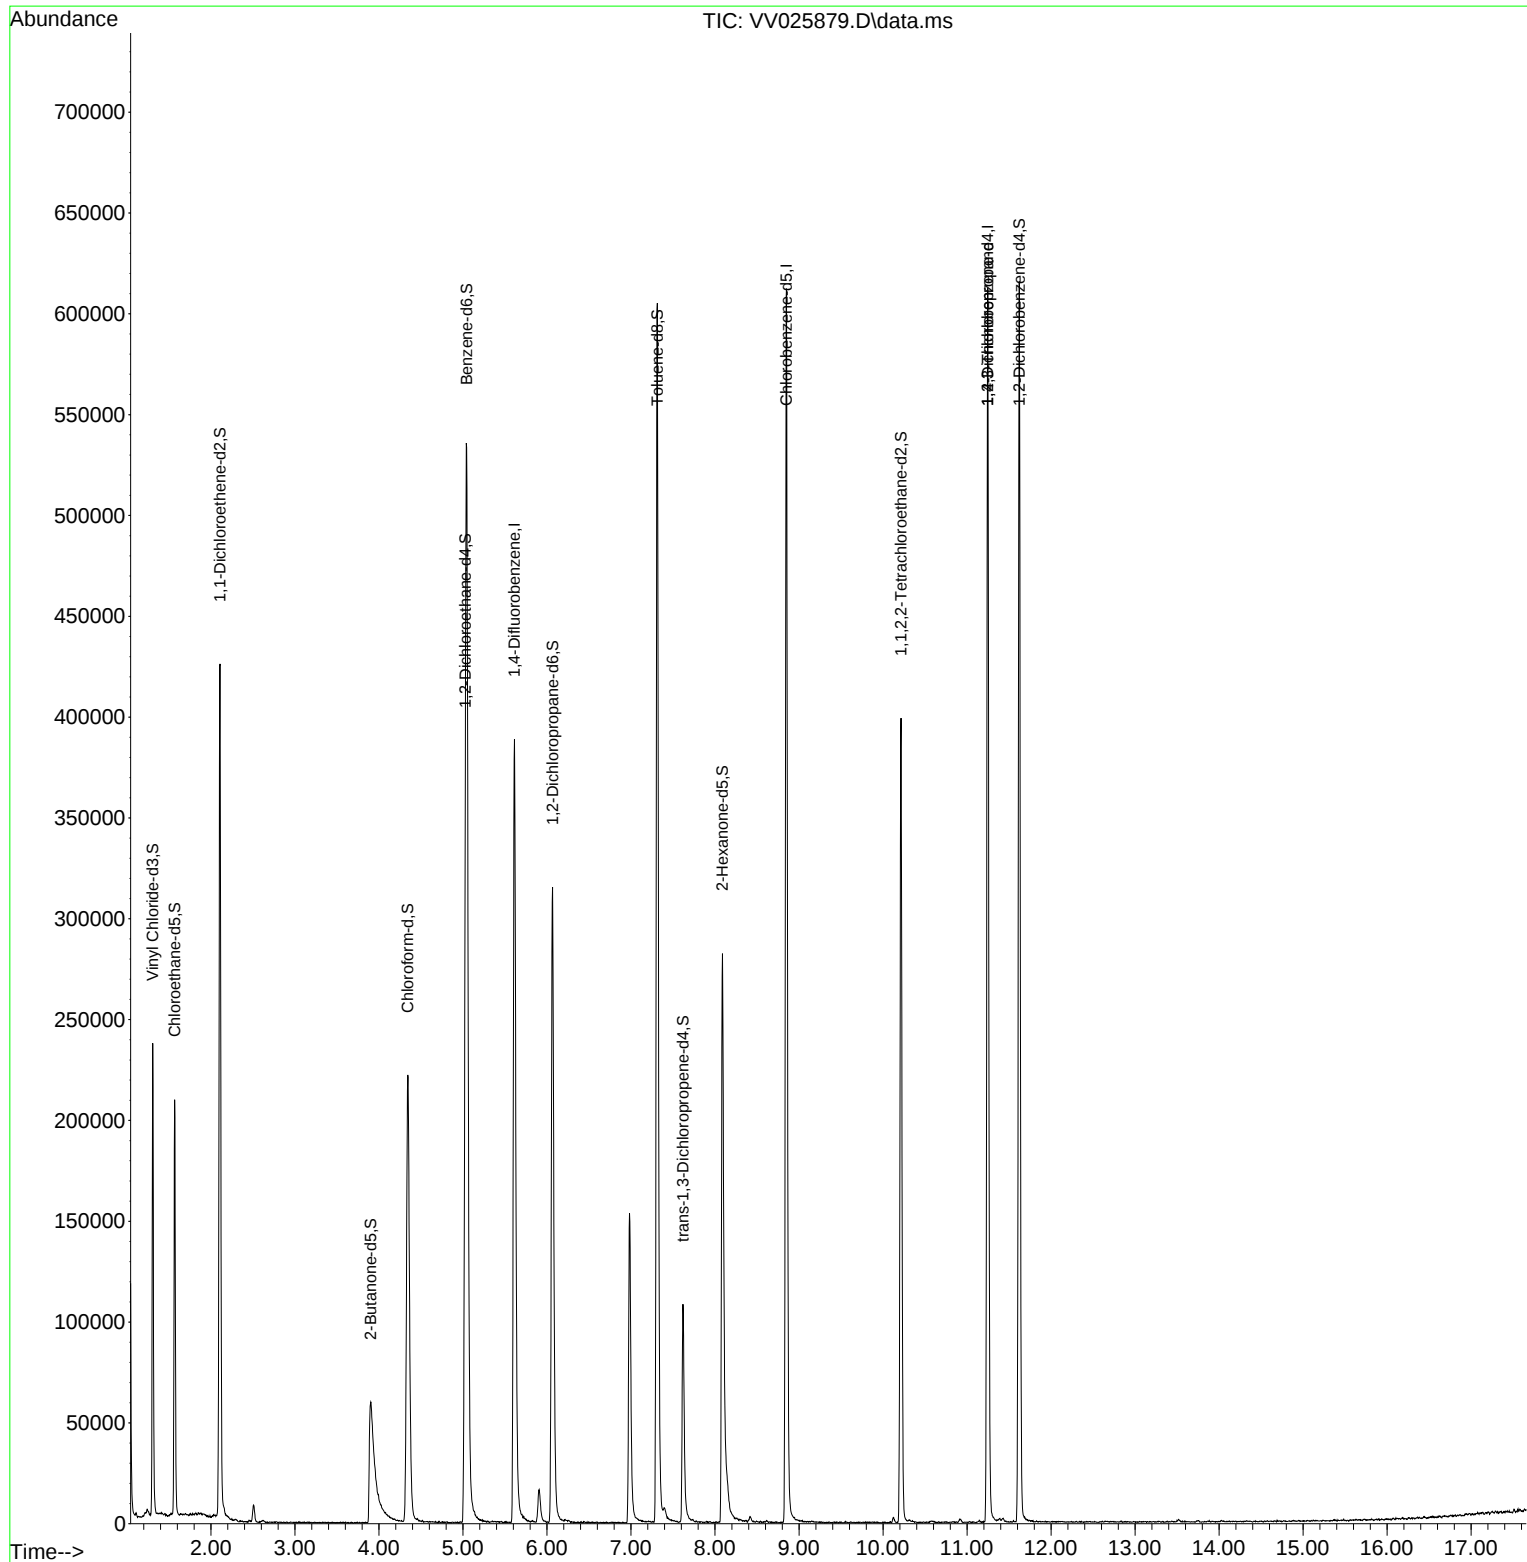

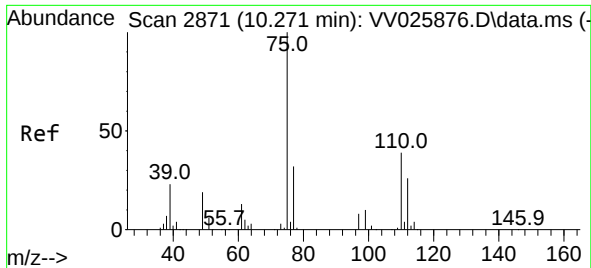

#61

1,2,3-Trichloropropane

Concen: 6.335 ug/L

RT: 11.246 min Scan# 31

Delta R.T. 0.974 min

Lab File: VV025879.D


Acq: 12 May 2022 13:55

Instrument :

MSVOA_V

ClientSampleId :

DBSL2ME

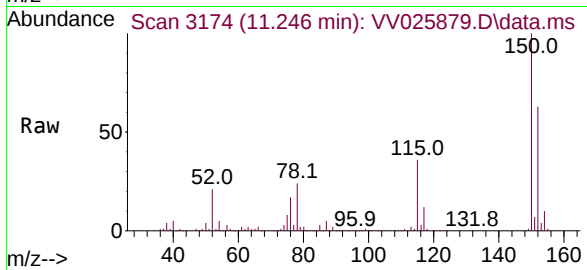

Tgt Ion: 75 Resp: 19460

Ion Ratio Lower Upper

75 100

77 31.4 25.3 37.9

110 2.4 32.3 48.5#

