

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW051222\
 Data File : VW025881.D
 Acq On : 12 May 2022 14:45
 Operator : SY/MD
 Sample : N2714-05ME
 Misc : 5.49g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW2X6ME

Quant Time: May 13 07:09:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 13 07:07:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	329145	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	327509	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	150420	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	153051	36.030	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	72.060%
7) Chloroethane-d5	1.568	69	129964	34.839	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	69.680%#
11) 1,1-Dichloroethene-d2	2.108	63	231547	31.166	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	62.340%
21) 2-Butanone-d5	3.905	46	144668	79.457	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	79.460%
24) Chloroform-d	4.346	84	239056	40.291	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.580%
26) 1,2-Dichloroethane-d4	5.031	65	152318	42.477	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.960%
32) Benzene-d6	5.047	84	483091	42.312	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.620%
36) 1,2-Dichloropropane-d6	6.066	67	152799	43.573	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	87.140%
41) Toluene-d8	7.313	98	410263	39.000	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	78.000%#
43) trans-1,3-Dichloroprop...	7.619	79	63810	40.763	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.520%
47) 2-Hexanone-d5	8.088	63	108643	84.504	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	84.500%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	198494	42.445	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	84.900%
66) 1,2-Dichlorobenzene-d4	11.622	152	153635	46.562	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.120%
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.108	101	2180	0.690	ug/L #	22
61) 1,2,3-Trichloropropane	11.246	75	17808	5.981	ug/L #	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
Data File : VV025881.D
Acq On : 12 May 2022 14:45
Operator : SY/MD
Sample : N2714-05ME
Misc : 5.49g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW2X6ME

Quant Time: May 13 07:09:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 13 07:07:32 2022
Response via : Initial Calibration




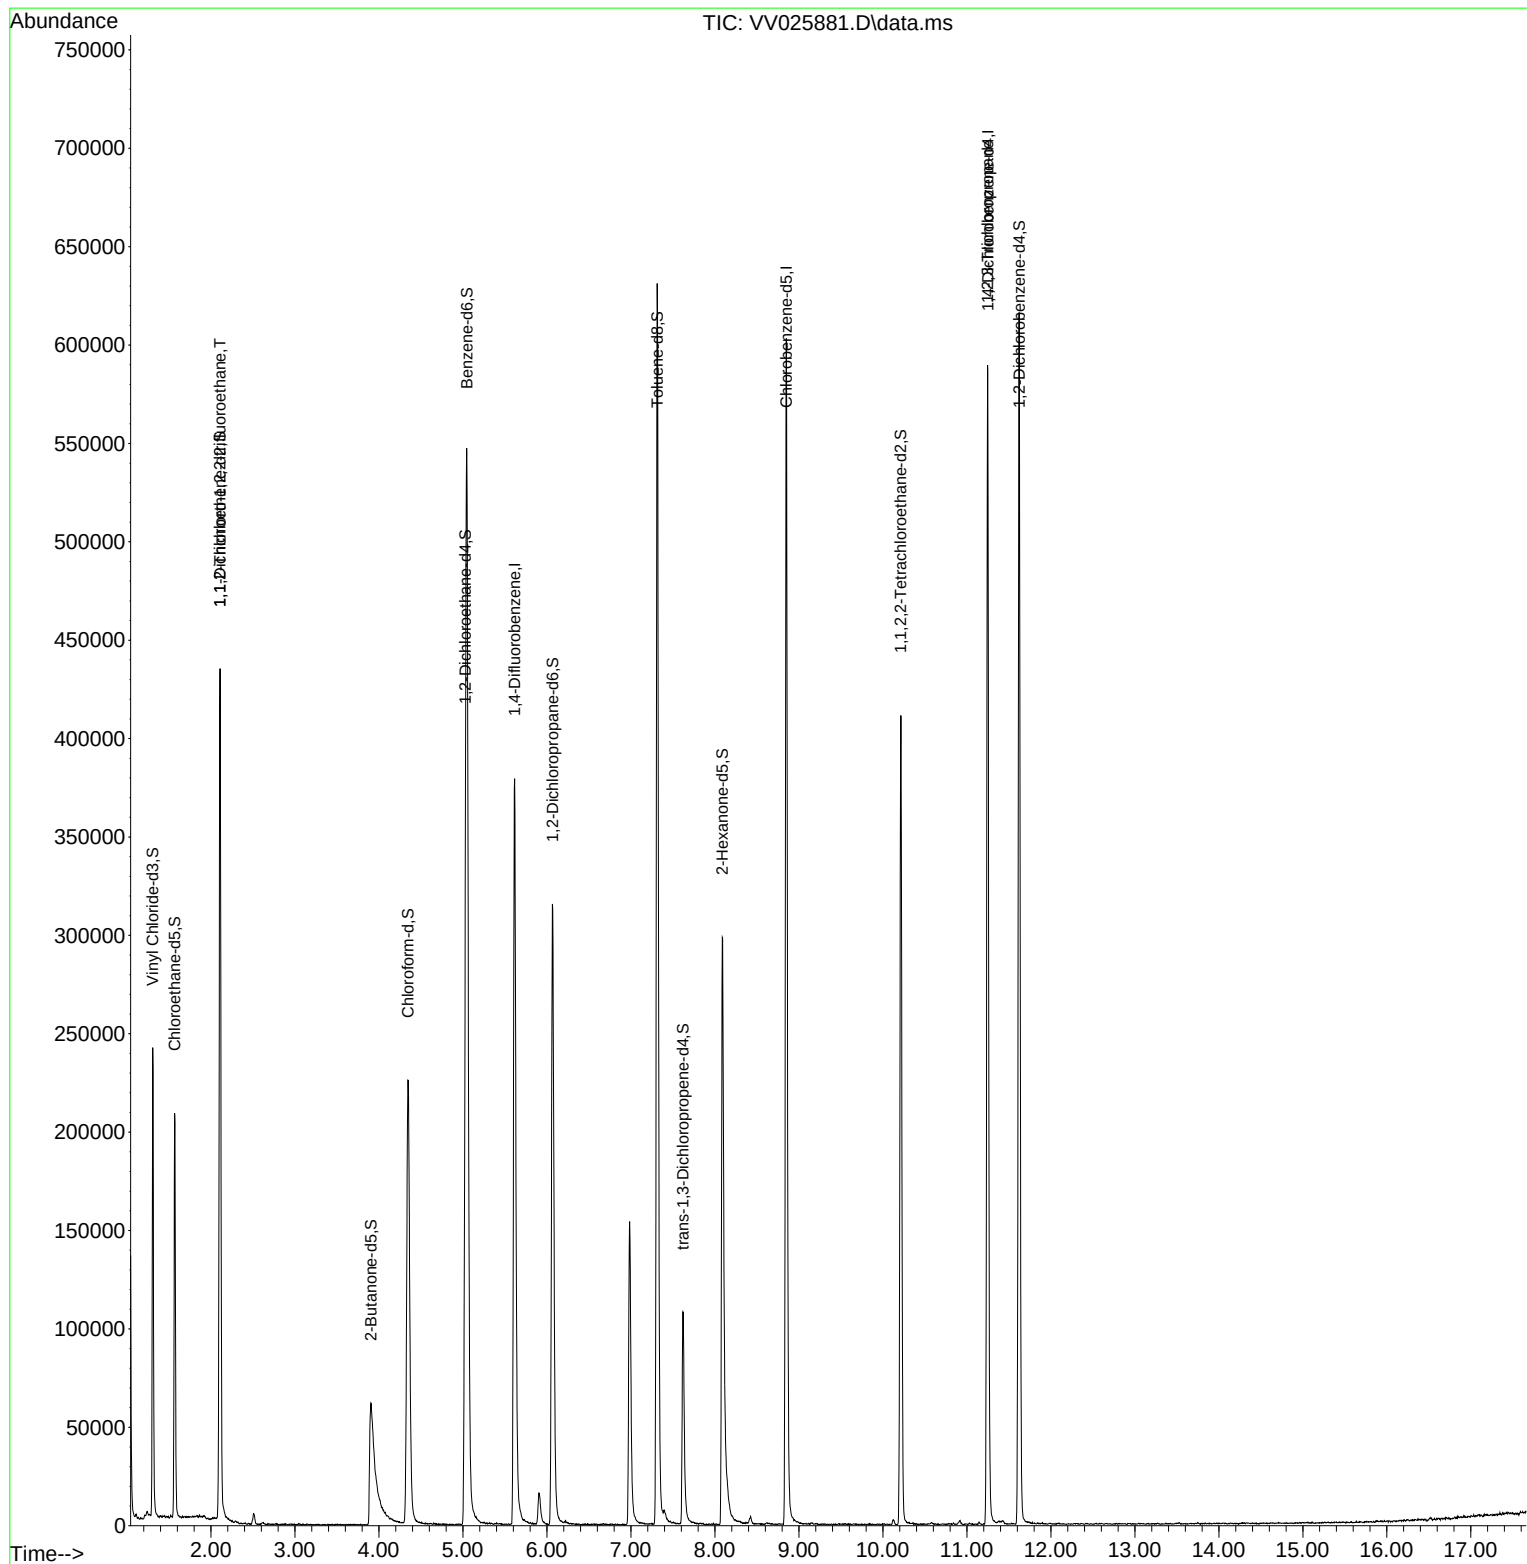


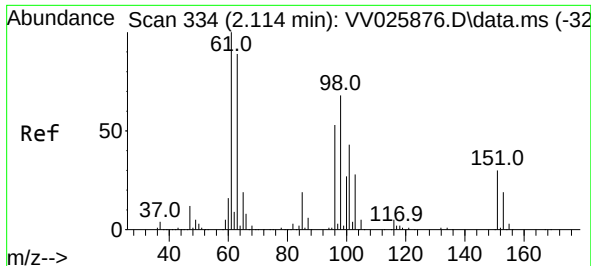

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.690 ug/L
 RT: 2.108 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: VV025881.D
 Acq: 12 May 2022 14:45

Instrument :
 MSVOA_V
 ClientSampleId :
 EW2X6ME

Tgt Ion:101 Resp: 2180
 Ion Ratio Lower Upper
 101 100
 85 0.0 34.6 51.8#
 151 0.0 54.3 81.5#

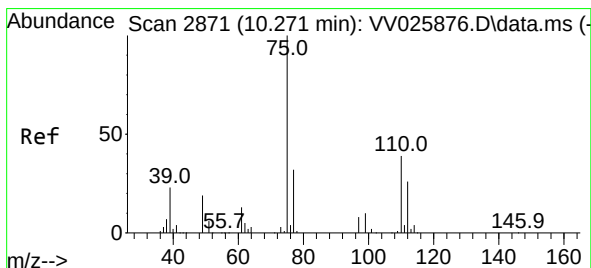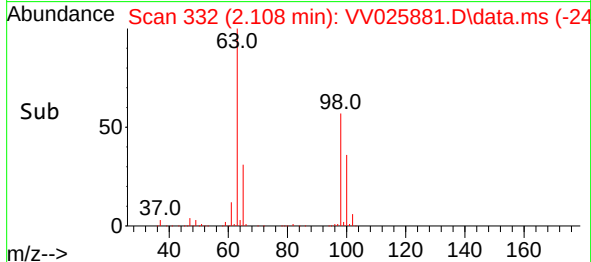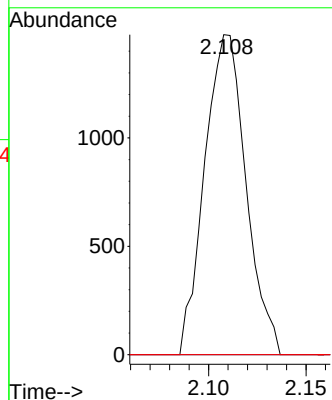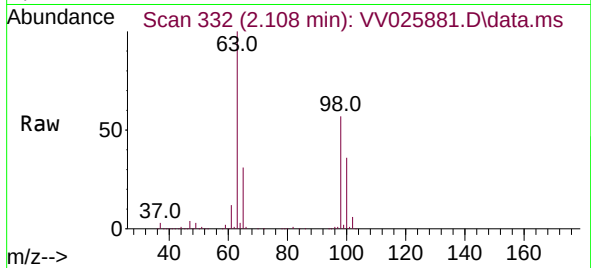

#61
 1,2,3-Trichloropropane
 Concen: 5.981 ug/L
 RT: 11.246 min Scan# 3174
 Delta R.T. 0.974 min
 Lab File: VV025881.D
 Acq: 12 May 2022 14:45

Tgt Ion: 75 Resp: 17808
 Ion Ratio Lower Upper
 75 100
 77 32.5 25.3 37.9
 110 2.8 32.3 48.5#

