

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW051222\
 Data File : VW025882.D
 Acq On : 12 May 2022 15:09
 Operator : SY/MD
 Sample : N2714-06ME
 Misc : 3.55g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW2X7ME

Quant Time: May 13 07:09:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 13 07:07:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	316078	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	315279	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	143756	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	147467	36.150	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	72.300%		
7) Chloroethane-d5	1.568	69	125285	34.973	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	69.940%#		
11) 1,1-Dichloroethene-d2	2.108	63	221667	31.070	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	62.140%		
21) 2-Butanone-d5	3.908	46	169994	97.227	ug/L	0.01
Spiked Amount 100.000	Range 40 - 130		Recovery =	97.230%		
24) Chloroform-d	4.349	84	230616	40.475	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	80.960%		
26) 1,2-Dichloroethane-d4	5.031	65	151201	43.909	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.820%		
32) Benzene-d6	5.050	84	459369	41.795	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	83.580%		
36) 1,2-Dichloropropane-d6	6.069	67	148855	44.095	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	88.180%		
41) Toluene-d8	7.317	98	394749	38.980	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	77.960%#		
43) trans-1,3-Dichloroprop...	7.622	79	61584	40.867	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	81.740%		
47) 2-Hexanone-d5	8.092	63	113824	91.968	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	91.970%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	197701	43.916	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	87.840%		
66) 1,2-Dichlorobenzene-d4	11.622	152	148549	47.108	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.220%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.985	75	3927	1.033	ug/L #	81
61) 1,2,3-Trichloropropane	11.246	75	17761	6.242	ug/L #	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
Data File : VV025882.D
Acq On : 12 May 2022 15:09
Operator : SY/MD
Sample : N2714-06ME
Misc : 3.55g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW2X7ME

Quant Time: May 13 07:09:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 13 07:07:32 2022
Response via : Initial Calibration

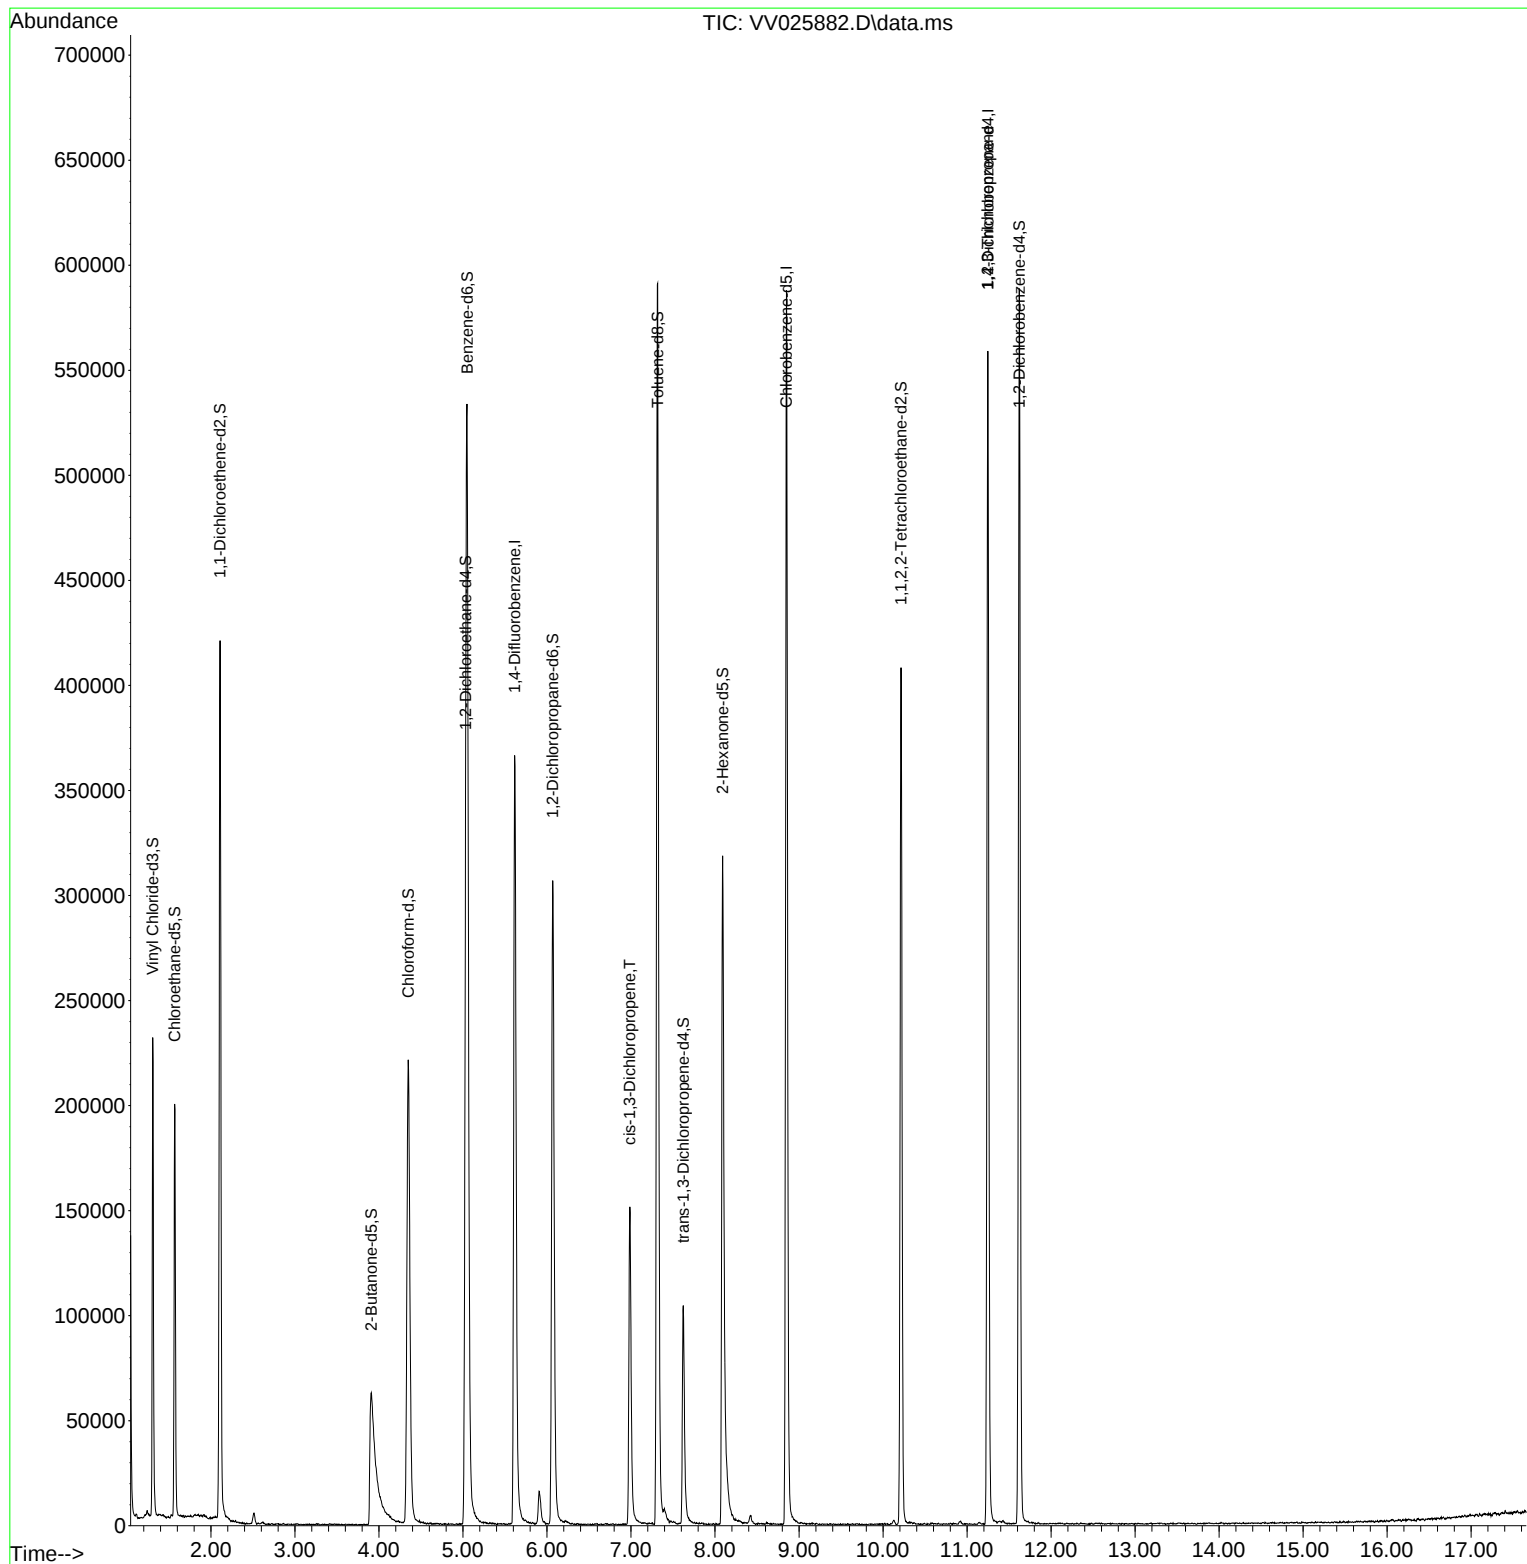

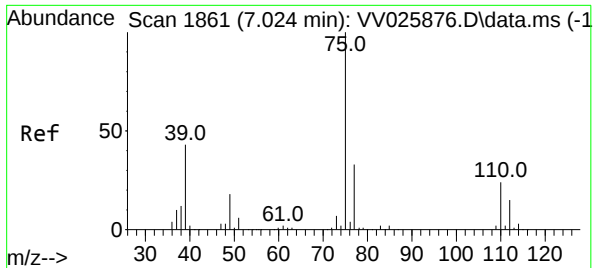

#39

cis-1,3-Dichloropropene

Concen: 1.033 ug/L

RT: 6.985 min Scan# 11

Delta R.T. -0.038 min

Lab File: VV025882.D

Acq: 12 May 2022 15:09

Instrument :

MSVOA_V

ClientSampleId :





EW2X7ME

Tgt Ion: 75 Resp: 3927

Ion Ratio Lower Upper

75 100

77 42.6 22.4 41.6#

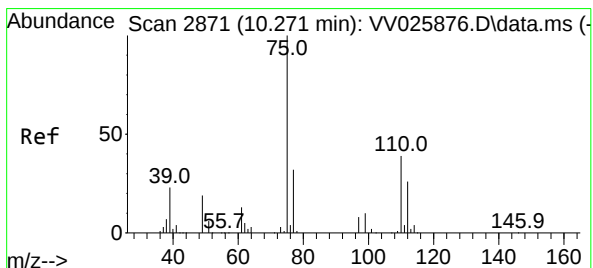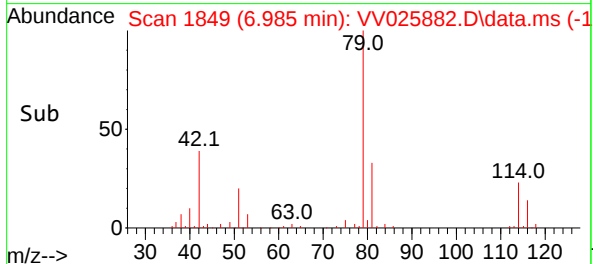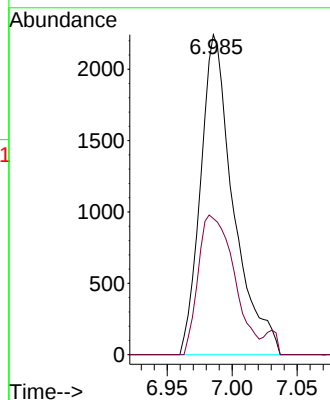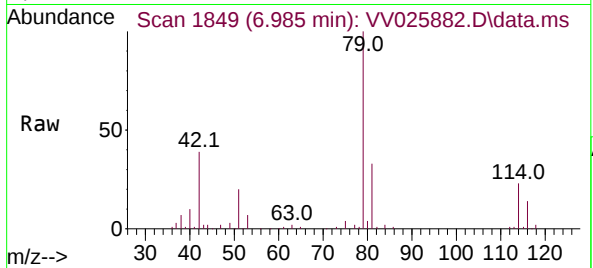

#61

1,2,3-Trichloropropane

Concen: 6.242 ug/L

RT: 11.246 min Scan# 3174

Delta R.T. 0.974 min

Lab File: VV025882.D

Acq: 12 May 2022 15:09

Tgt Ion: 75 Resp: 17761

Ion Ratio Lower Upper

75 100

77 31.2 25.3 37.9

110 2.5 32.3 48.5#

