

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW051222\
 Data File : VW025884.D
 Acq On : 12 May 2022 15:56
 Operator : SY/MD
 Sample : N2713-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBSK3

Quant Time: May 13 07:09:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 13 07:07:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	296071	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	301180	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	132890	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	142978	37.418	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	74.840%		
7) Chloroethane-d5	1.568	69	123468	36.795	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	73.580%		
11) 1,1-Dichloroethene-d2	2.108	63	217371	32.526	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	65.060%		
21) 2-Butanone-d5	3.905	46	157802	96.353	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	96.350%		
24) Chloroform-d	4.349	84	226908	42.516	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.040%		
26) 1,2-Dichloroethane-d4	5.031	65	148946	46.177	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.360%		
32) Benzene-d6	5.050	84	455537	43.386	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.780%		
36) 1,2-Dichloropropane-d6	6.069	67	149400	46.328	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	92.660%		
41) Toluene-d8	7.313	98	388787	40.189	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	80.380%		
43) trans-1,3-Dichloroprop...	7.622	79	61325	42.600	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	85.200%		
47) 2-Hexanone-d5	8.091	63	115931	98.055	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	98.060%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	196887	45.782	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	91.560%		
66) 1,2-Dichlorobenzene-d4	11.622	152	146764	50.347	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	100.700%		
Target Compounds						Qvalue
35) Methylcyclohexane	6.069	83	36072	9.080	ug/L #	20
61) 1,2,3-Trichloropropane	11.246	75	16651	6.330	ug/L #	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
Data File : VV025884.D
Acq On : 12 May 2022 15:56
Operator : SY/MD
Sample : N2713-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBSK3

Quant Time: May 13 07:09:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 13 07:07:32 2022
Response via : Initial Calibration




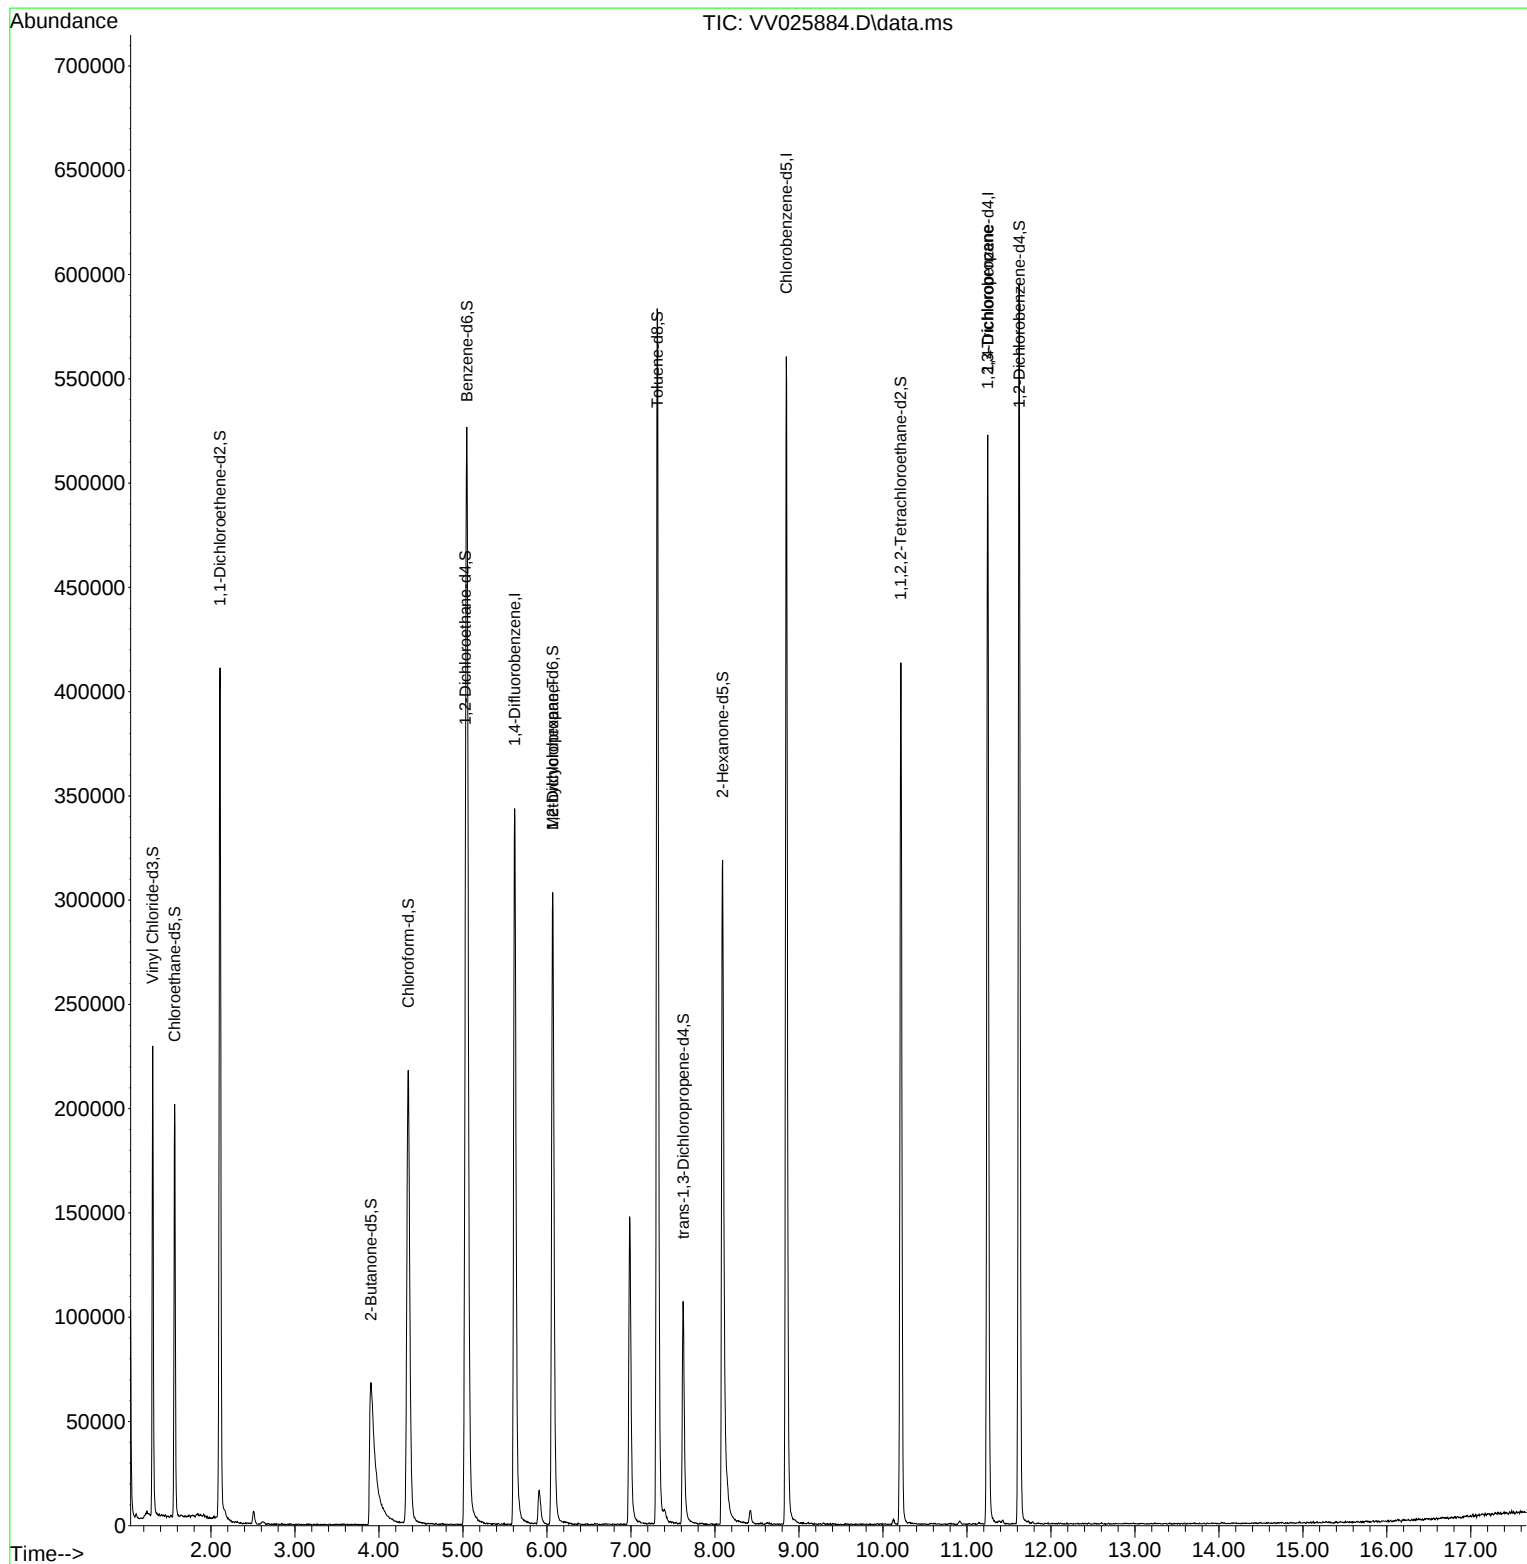


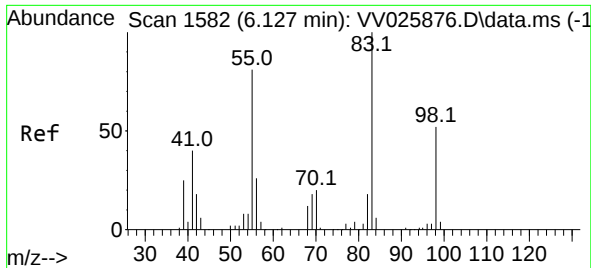

#35
Methylcyclohexane
Concen: 9.080 ug/L
RT: 6.069 min Scan# 11
Delta R.T. -0.058 min
Lab File: VV025884.D
Acq: 12 May 2022 15:56

Instrument :
MSVOA_V
ClientSampleId :
DBSK3

Tgt Ion: 83 Resp: 36072
Ion Ratio Lower Upper
83 100
55 0.5 58.6 87.8#
98 1.4 39.1 58.7#

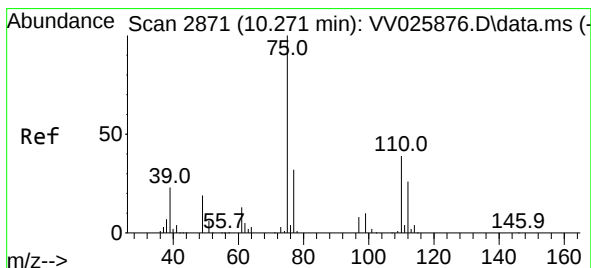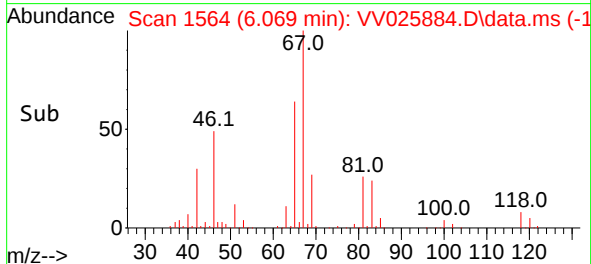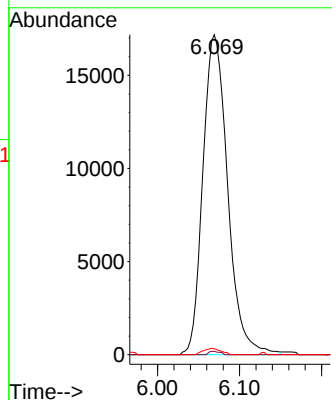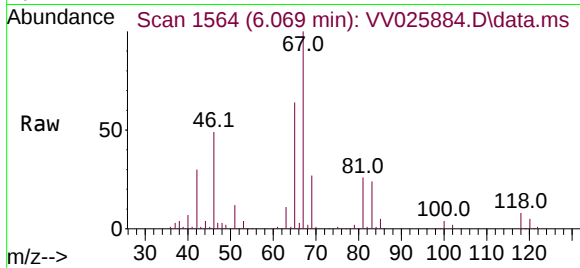

#61
1,2,3-Trichloropropane
Concen: 6.330 ug/L
RT: 11.246 min Scan# 3174
Delta R.T. 0.974 min
Lab File: VV025884.D
Acq: 12 May 2022 15:56

Tgt Ion: 75 Resp: 16651
Ion Ratio Lower Upper
75 100
77 31.4 25.3 37.9
110 3.2 32.3 48.5#

