

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
 Data File : VV025877.D
 Acq On : 12 May 2022 12:57
 Operator : SY/MD
 Sample : VV0512MBL01
 Misc : 5.00g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK213

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

Signal : TIC: VV025877.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	97	rVB	265977	273330	18.09%	2.433%
2	1.568	157	164	176	rBV	222234	250776	16.60%	2.232%
3	2.108	322	332	353	rVB	468655	673957	44.61%	5.999%
4	2.600	482	485	488	rBV2	376	175	0.01%	0.002%
5	2.744	527	530	532	rBV2	542	279	0.02%	0.002%
6	2.854	561	564	567	rBV3	355	309	0.02%	0.003%
7	2.889	572	575	579	rVV	506	392	0.03%	0.003%
8	3.050	623	625	629	rBV2	430	234	0.02%	0.002%
9	3.069	629	631	635	rVV2	271	192	0.01%	0.002%
10	3.156	656	658	662	rVB	267	153	0.01%	0.001%
11	3.182	662	666	669	rBV2	356	331	0.02%	0.003%
12	3.227	678	680	684	rBV3	308	150	0.01%	0.001%
13	3.285	697	698	703	rVB2	283	152	0.01%	0.001%
14	3.307	703	705	708	rBV	340	237	0.02%	0.002%
15	3.326	708	711	715	rVB3	407	272	0.02%	0.002%
16	3.358	715	721	722	rBV3	502	412	0.03%	0.004%
17	3.487	758	761	763	rVV2	240	136	0.01%	0.001%
18	3.571	784	787	789	rBV	306	175	0.01%	0.002%
19	3.651	809	812	813	rBV2	293	171	0.01%	0.002%
20	3.690	822	824	827	rVV	404	265	0.02%	0.002%
21	3.709	827	830	832	rVV2	507	240	0.02%	0.002%
22	3.748	835	842	847	rBV2	664	684	0.05%	0.006%
23	3.789	853	855	858	rVV2	401	193	0.01%	0.002%
24	3.905	879	891	925	rBV2	60576	263587	17.45%	2.346%
25	4.342	1013	1027	1054	rVB	239469	588906	38.98%	5.242%
26	4.760	1155	1157	1160	rVB2	478	218	0.01%	0.002%
27	4.825	1176	1177	1181	rVB	342	178	0.01%	0.002%
28	4.850	1181	1185	1188	rVB3	442	352	0.02%	0.003%
29	4.876	1191	1193	1196	rBV	357	186	0.01%	0.002%
30	5.043	1226	1245	1288	rBV2	583448	1510707	100.00%	13.448%
31	5.326	1330	1333	1337	rBV5	461	386	0.03%	0.003%
32	5.391	1351	1353	1354	rBV5	631	253	0.02%	0.002%
33	5.445	1367	1370	1372	rBV	367	184	0.01%	0.002%
34	5.548	1398	1402	1403	rBV2	282	196	0.01%	0.002%
35	5.567	1407	1408	1410	rBV	552	263	0.02%	0.002%
36	5.612	1410	1422	1458	rVV	393824	804319	53.24%	7.160%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
 Data File : VV025877.D
 Acq On : 12 May 2022 12:57
 Operator : SY/MD
 Sample : VV0512MBL01
 Misc : 5.00g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK213

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

37	5.905	1501	1513	1528	rBV2	14382	31345	2.07%	0.279%
38	6.011	1544	1546	1547	rBV2	701	283	0.02%	0.003%
39	6.066	1549	1563	1594	rVV	329154	684350	45.30%	6.092%
40	6.300	1634	1636	1639	rBV4	384	331	0.02%	0.003%
41	6.352	1647	1652	1655	rBV3	456	346	0.02%	0.003%
42	6.368	1655	1657	1660	rBV2	303	160	0.01%	0.001%
43	6.407	1668	1669	1671	rBV2	327	149	0.01%	0.001%
44	6.442	1677	1680	1681	rBV2	345	174	0.01%	0.002%
45	6.538	1707	1710	1713	rBV	350	293	0.02%	0.003%
46	6.564	1716	1718	1720	rVB2	357	160	0.01%	0.001%
47	6.628	1735	1738	1740	rBV3	227	190	0.01%	0.002%
48	6.657	1745	1747	1748	rBV	349	129	0.01%	0.001%
49	6.690	1755	1757	1762	rVB3	367	269	0.02%	0.002%
50	6.722	1762	1767	1776	rVB3	460	677	0.04%	0.006%
51	6.763	1776	1780	1783	rBV3	409	287	0.02%	0.003%
52	6.879	1811	1816	1821	rBV4	297	395	0.03%	0.004%
53	6.940	1831	1835	1838	rBV4	295	263	0.02%	0.002%
54	6.982	1838	1848	1871	rBV	170020	310477	20.55%	2.764%
55	7.201	1913	1916	1918	rBV2	735	502	0.03%	0.004%
56	7.313	1938	1951	1971	rBV	663266	1157887	76.65%	10.307%
57	7.619	2036	2046	2069	rBV	117628	213738	14.15%	1.903%
58	7.802	2101	2103	2106	rBV3	466	283	0.02%	0.003%
59	7.821	2107	2109	2116	rVV4	803	623	0.04%	0.006%
60	7.879	2124	2127	2132	rVB2	551	389	0.03%	0.003%
61	7.908	2134	2136	2140	rVB2	280	172	0.01%	0.002%
62	7.976	2155	2157	2160	rVB2	708	427	0.03%	0.004%
63	8.024	2166	2172	2174	rBV3	504	553	0.04%	0.005%
64	8.088	2178	2192	2223	rBV	320990	663811	43.94%	5.909%
65	8.519	2324	2326	2327	rBV	370	129	0.01%	0.001%
66	8.712	2381	2386	2389	rVV3	539	526	0.03%	0.005%
67	8.754	2397	2399	2403	rBV5	469	305	0.02%	0.003%
68	8.779	2404	2407	2411	rBV3	542	479	0.03%	0.004%
69	8.847	2417	2428	2459	rBV	626452	1032453	68.34%	9.191%
70	9.214	2536	2542	2543	rBV3	621	482	0.03%	0.004%
71	9.374	2589	2592	2594	rBV	268	215	0.01%	0.002%
72	9.445	2609	2614	2617	rVV3	469	417	0.03%	0.004%
73	9.464	2617	2620	2623	rBV2	272	167	0.01%	0.001%
74	9.760	2710	2712	2718	rBV3	364	317	0.02%	0.003%
75	9.937	2761	2767	2773	rVB4	1573	1952	0.13%	0.017%
76	10.021	2790	2793	2796	rBV2	352	226	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
 Data File : VV025877.D
 Acq On : 12 May 2022 12:57
 Operator : SY/MD
 Sample : VV0512MBL01
 Misc : 5.00g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK213

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

77	10.066	2805	2807	2809	rBV	433	186	0.01%	0.002%
78	10.127	2817	2826	2835	rVB7	2295	4005	0.27%	0.036%
79	10.213	2841	2853	2878	rBV	439799	693402	45.90%	6.173%
80	10.439	2921	2923	2926	rBV2	355	259	0.02%	0.002%
81	10.509	2943	2945	2948	rBV2	295	165	0.01%	0.001%
82	10.683	2990	2999	3004	rBV3	593	846	0.06%	0.008%
83	10.705	3004	3006	3010	rBV	278	152	0.01%	0.001%
84	10.802	3033	3036	3039	rVV	628	496	0.03%	0.004%
85	10.831	3043	3045	3046	rBV	308	150	0.01%	0.001%
86	10.876	3057	3059	3064	rVB5	396	305	0.02%	0.003%
87	10.921	3064	3073	3083	rVB6	3459	5391	0.36%	0.048%
88	11.027	3104	3106	3108	rBV	349	182	0.01%	0.002%
89	11.143	3137	3142	3148	rVB4	1468	1311	0.09%	0.012%
90	11.188	3148	3156	3162	rBV5	3387	4375	0.29%	0.039%
91	11.246	3163	3174	3205	rVV	624011	964356	63.83%	8.585%
92	11.512	3255	3257	3259	rBV2	433	159	0.01%	0.001%
93	11.622	3279	3291	3313	rBV	658165	1039719	68.82%	9.255%
94	11.847	3353	3361	3364	rBV4	1005	1210	0.08%	0.011%
95	12.647	3602	3610	3617	rBV7	2916	4241	0.28%	0.038%
96	12.741	3637	3639	3644	rVB	478	273	0.02%	0.002%
97	13.114	3751	3755	3758	rBV	343	307	0.02%	0.003%
98	13.265	3796	3802	3809	rBV5	3908	5467	0.36%	0.049%
99	13.503	3868	3876	3881	rBV3	12710	18714	1.24%	0.167%
100	13.741	3943	3950	3961	rBV6	5515	8625	0.57%	0.077%

Sum of corrected areas: 11233577




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
Data File : VV025877.D
Acq On : 12 May 2022 12:57
Operator : SY/MD
Sample : VV0512MBL01
Misc : 5.00g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK213

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

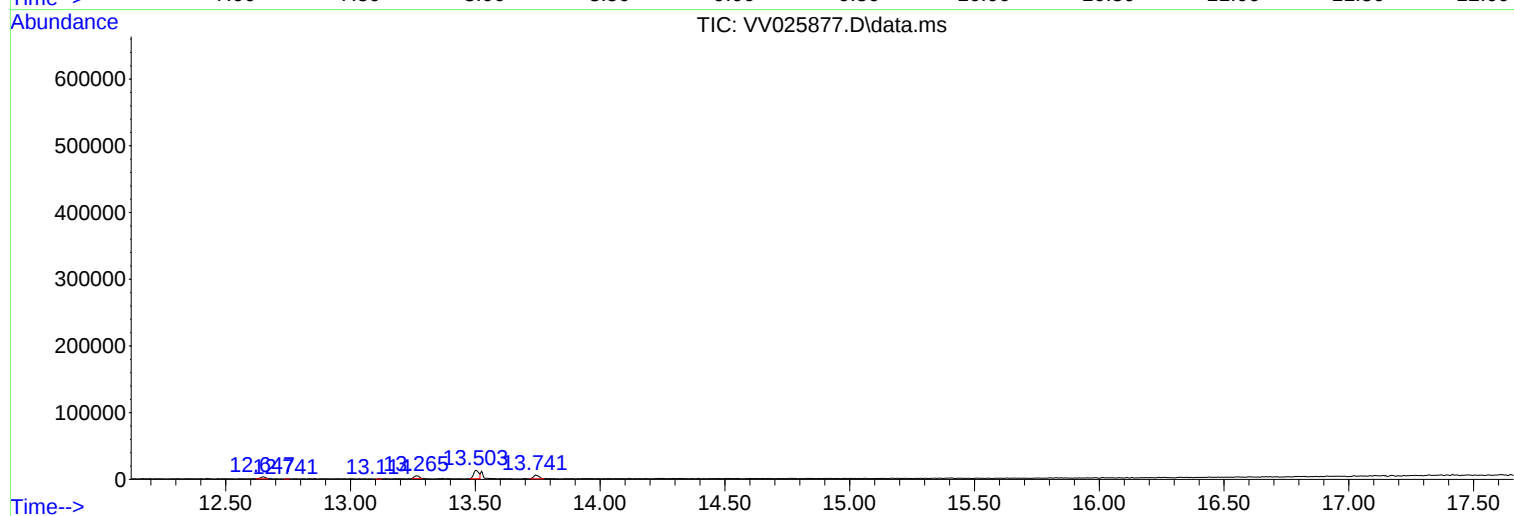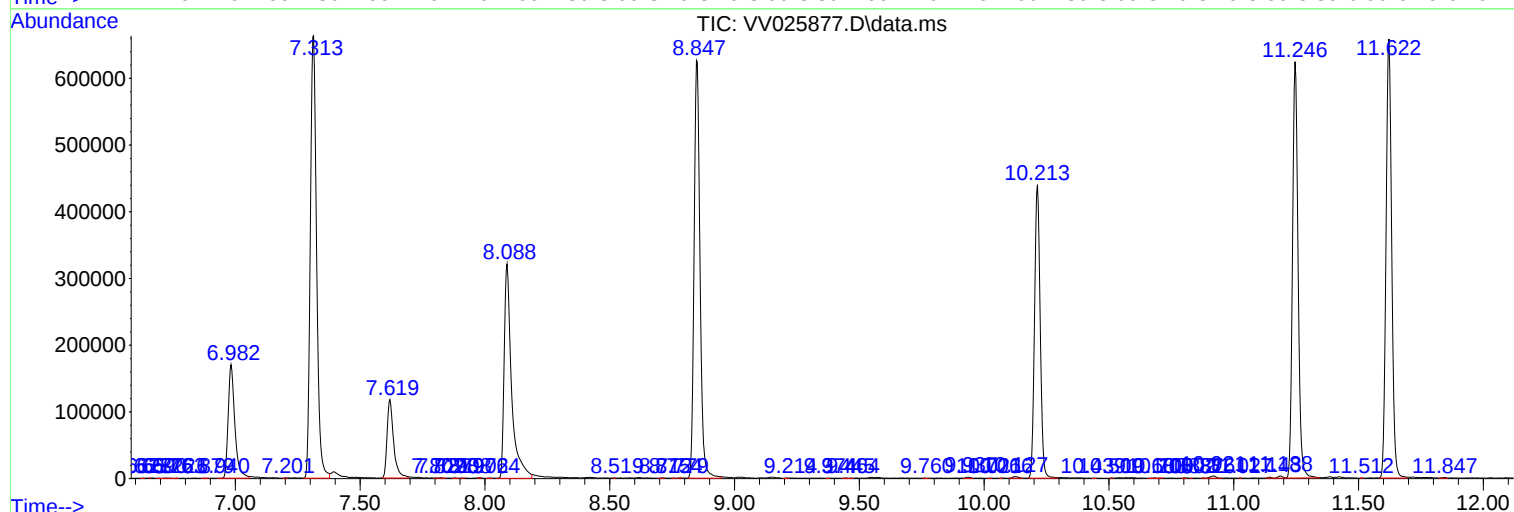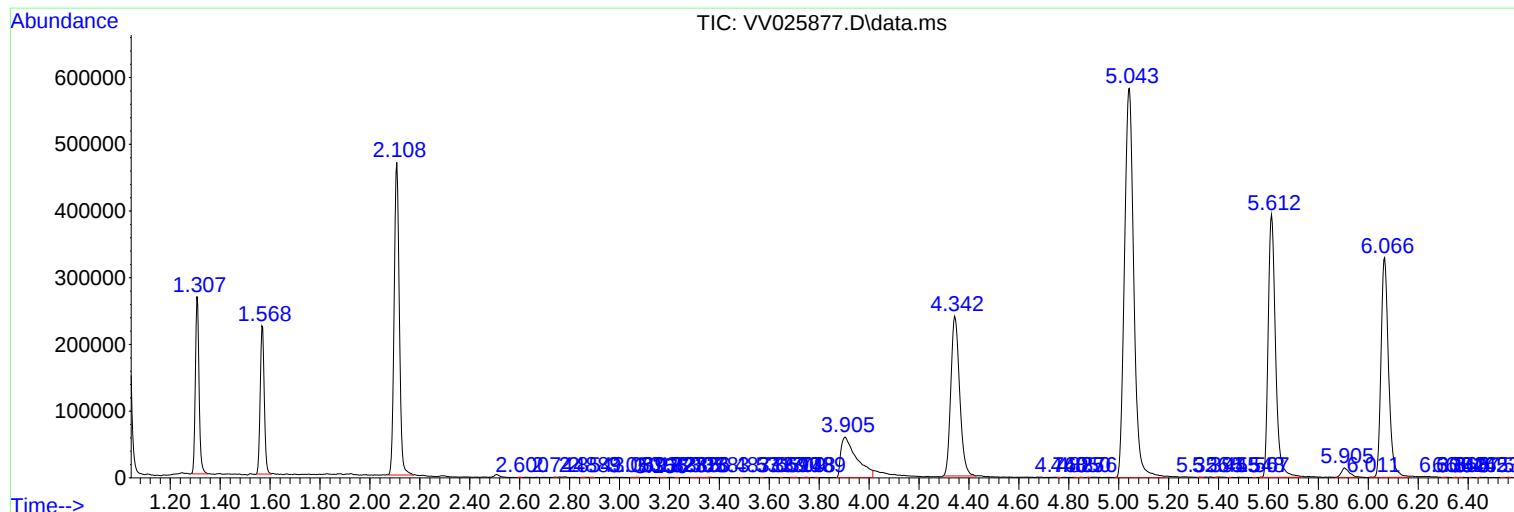

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
Data File : VV025877.D
Acq On : 12 May 2022 12:57
Operator : SY/MD
Sample : VV0512MBL01
Misc : 5.00g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK213

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
Data File : VV025877.D
Acq On : 12 May 2022 12:57
Operator : SY/MD
Sample : VV0512MBL01
Misc : 5.00g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK213

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc