

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
 Data File : VV025878.D
 Acq On : 12 May 2022 13:21
 Operator : SY/MD
 Sample : VV0512WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK214

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

Signal : TIC: VV025878.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	103	rVB	241657	255286	17.94%	2.411%
2	1.571	157	165	181	rVB	209713	239999	16.86%	2.267%
3	2.108	322	332	359	rVB	446618	644777	45.31%	6.090%
4	2.513	450	458	464	rBV4	3151	4689	0.33%	0.044%
5	2.574	474	477	483	rBV2	405	326	0.02%	0.003%
6	2.648	497	500	502	rVB2	528	305	0.02%	0.003%
7	2.703	513	517	520	rBV2	567	435	0.03%	0.004%
8	2.757	532	534	537	rVB	405	176	0.01%	0.002%
9	2.786	537	543	549	rVB3	690	682	0.05%	0.006%
10	2.822	549	554	556	rBV3	230	228	0.02%	0.002%
11	2.905	578	580	583	rBV3	339	226	0.02%	0.002%
12	2.954	592	595	598	rBV3	443	368	0.03%	0.003%
13	3.198	668	671	673	rBV	293	174	0.01%	0.002%
14	3.307	699	705	709	rBV3	319	297	0.02%	0.003%
15	3.327	709	711	714	rBV2	479	252	0.02%	0.002%
16	3.362	720	722	729	rVB2	226	214	0.02%	0.002%
17	3.490	760	762	766	rVB2	326	179	0.01%	0.002%
18	3.519	766	771	773	rBV3	406	380	0.03%	0.004%
19	3.600	795	796	798	rBV	340	171	0.01%	0.002%
20	3.635	806	807	812	rBV2	388	207	0.01%	0.002%
21	3.677	817	820	823	rBV2	300	195	0.01%	0.002%
22	3.699	823	827	832	rBV2	247	232	0.02%	0.002%
23	3.767	846	848	851	rBV	309	201	0.01%	0.002%
24	3.780	851	852	857	rVB3	413	211	0.01%	0.002%
25	3.905	880	891	933	rBV	57992	269436	18.93%	2.545%
26	4.349	1013	1029	1058	rBV	231454	579021	40.69%	5.469%
27	4.580	1098	1101	1107	rBV4	656	563	0.04%	0.005%
28	4.664	1125	1127	1131	rBV3	499	349	0.02%	0.003%
29	4.712	1140	1142	1146	rVB2	449	237	0.02%	0.002%
30	4.767	1157	1159	1162	rBV	247	200	0.01%	0.002%
31	4.806	1167	1171	1172	rBV	379	204	0.01%	0.002%
32	4.886	1192	1196	1199	rBV3	439	299	0.02%	0.003%
33	4.921	1204	1207	1211	rVB2	332	223	0.02%	0.002%
34	5.047	1229	1246	1272	rBV2	556624	1423132	100.00%	13.441%
35	5.310	1327	1328	1333	rBV2	321	265	0.02%	0.003%
36	5.413	1357	1360	1363	rBV2	838	631	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
 Data File : VV025878.D
 Acq On : 12 May 2022 13:21
 Operator : SY/MD
 Sample : VV0512WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK214

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

37	5.474	1373	1379	1381	rBV3	392	424	0.03%	0.004%
38	5.513	1389	1391	1393	rBV2	513	273	0.02%	0.003%
39	5.532	1395	1397	1400	rVB2	688	334	0.02%	0.003%
40	5.548	1400	1402	1406	rBV3	377	215	0.02%	0.002%
41	5.571	1406	1409	1411	rBV	395	258	0.02%	0.002%
42	5.616	1411	1423	1455	rBV	364035	741947	52.13%	7.007%
43	5.841	1491	1493	1495	rBV2	527	214	0.02%	0.002%
44	5.908	1503	1514	1540	rVB2	13669	33599	2.36%	0.317%
45	5.998	1540	1542	1545	rBV2	537	316	0.02%	0.003%
46	6.069	1549	1564	1595	rBV	316548	662728	46.57%	6.259%
47	6.314	1638	1640	1645	rBV3	344	363	0.03%	0.003%
48	6.336	1645	1647	1649	rVV3	484	218	0.02%	0.002%
49	6.384	1658	1662	1665	rBV3	394	369	0.03%	0.003%
50	6.490	1693	1695	1700	rVB2	480	341	0.02%	0.003%
51	6.516	1700	1703	1704	rBV2	577	316	0.02%	0.003%
52	6.526	1704	1706	1707	rVV	492	196	0.01%	0.002%
53	6.680	1751	1754	1757	rBV2	484	305	0.02%	0.003%
54	6.815	1795	1796	1799	rVB	360	167	0.01%	0.002%
55	6.834	1799	1802	1809	rVB2	426	477	0.03%	0.005%
56	6.986	1837	1849	1873	rBV	159217	296692	20.85%	2.802%
57	7.313	1939	1951	1971	rBV	629608	1093961	76.87%	10.332%
58	7.622	2037	2047	2071	rBV	108529	196849	13.83%	1.859%
59	7.966	2151	2154	2156	rBV2	401	169	0.01%	0.002%
60	8.037	2173	2176	2180	rBV2	423	245	0.02%	0.002%
61	8.092	2182	2193	2230	rBV	302068	634642	44.59%	5.994%
62	8.555	2334	2337	2338	rBV2	329	210	0.01%	0.002%
63	8.609	2352	2354	2355	rBV	658	261	0.02%	0.002%
64	8.690	2376	2379	2381	rBV	555	281	0.02%	0.003%
65	8.715	2385	2387	2390	rVV2	440	260	0.02%	0.002%
66	8.744	2393	2396	2398	rVB2	439	193	0.01%	0.002%
67	8.802	2412	2414	2417	rVB2	434	249	0.02%	0.002%
68	8.850	2417	2429	2460	rBV	590069	949245	66.70%	8.965%
69	9.114	2505	2511	2514	rBV5	780	880	0.06%	0.008%
70	9.272	2556	2560	2561	rBV2	403	297	0.02%	0.003%
71	9.333	2575	2579	2580	rBV	334	233	0.02%	0.002%
72	9.368	2588	2590	2593	rBV2	406	262	0.02%	0.002%
73	9.535	2640	2642	2645	rBV	266	169	0.01%	0.002%
74	9.741	2705	2706	2712	rVB2	317	178	0.01%	0.002%
75	9.789	2719	2721	2724	rVB2	382	181	0.01%	0.002%
76	9.876	2745	2748	2751	rBV2	449	212	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
 Data File : VV025878.D
 Acq On : 12 May 2022 13:21
 Operator : SY/MD
 Sample : VV0512WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK214

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

77	10.092	2813	2815	2818	rBV	351	222	0.02%	0.002%
78	10.124	2818	2825	2834	rBV4	2600	3852	0.27%	0.036%
79	10.214	2841	2853	2873	rBV	418848	662742	46.57%	6.259%
80	10.358	2896	2898	2902	rVB3	602	310	0.02%	0.003%
81	10.423	2916	2918	2920	rBV2	465	273	0.02%	0.003%
82	10.464	2924	2931	2935	rBV3	595	590	0.04%	0.006%
83	10.513	2941	2946	2947	rBV2	405	334	0.02%	0.003%
84	10.574	2960	2965	2967	rBV3	844	821	0.06%	0.008%
85	10.828	3041	3044	3045	rBV2	445	274	0.02%	0.003%
86	10.860	3051	3054	3056	rBV3	383	193	0.01%	0.002%
87	10.908	3065	3069	3070	rBV	1659	951	0.07%	0.009%
88	11.085	3120	3124	3125	rBV	354	182	0.01%	0.002%
89	11.140	3135	3141	3150	rVB5	1199	1492	0.10%	0.014%
90	11.181	3150	3154	3156	rBV2	1017	736	0.05%	0.007%
91	11.246	3163	3174	3194	rBV	570231	885266	62.21%	8.361%
92	11.622	3279	3291	3310	rBV	628615	979811	68.85%	9.254%
93	11.844	3356	3360	3362	rBV2	761	628	0.04%	0.006%
94	11.934	3386	3388	3389	rBV	486	195	0.01%	0.002%
95	12.368	3520	3523	3524	rBV2	360	221	0.02%	0.002%
96	12.590	3590	3592	3594	rBV	464	287	0.02%	0.003%
97	13.413	3844	3848	3850	rBV2	472	356	0.03%	0.003%
98	13.506	3873	3877	3886	rBV5	2601	3260	0.23%	0.031%
99	13.638	3915	3918	3922	rBV2	559	425	0.03%	0.004%
100	13.741	3945	3950	3951	rBV3	1379	1012	0.07%	0.010%


Sum of corrected areas: 10587932

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
Data File : VV025878.D
Acq On : 12 May 2022 13:21
Operator : SY/MD
Sample : VV0512WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK214

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

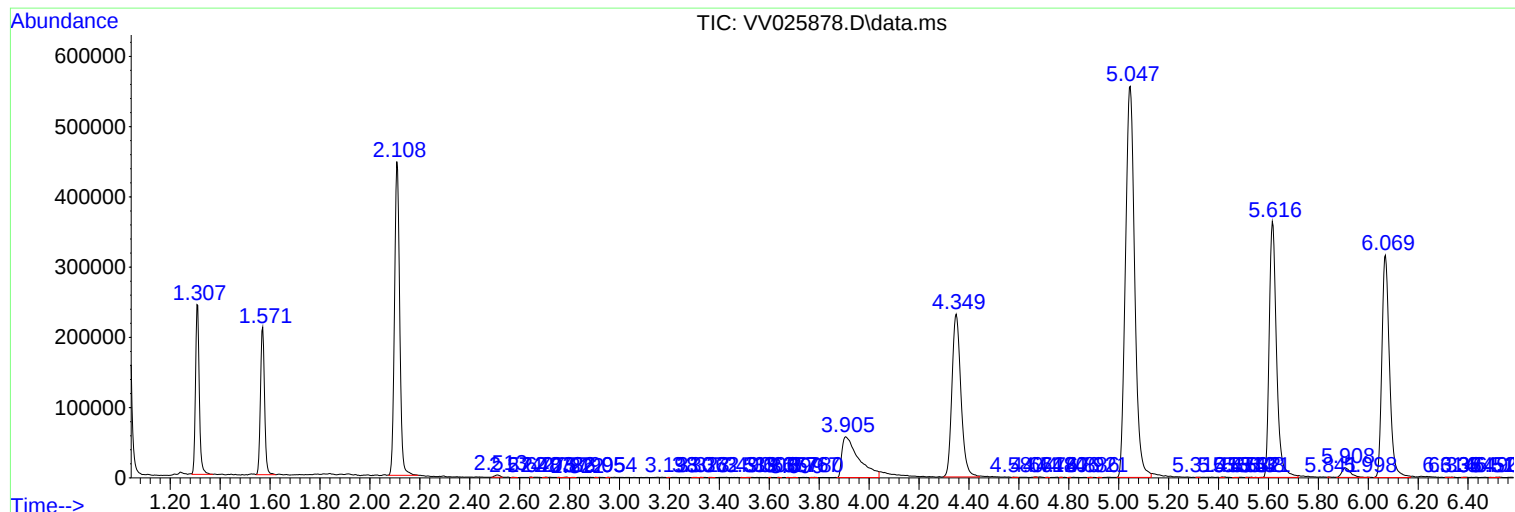

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
Data File : VV025878.D
Acq On : 12 May 2022 13:21
Operator : SY/MD
Sample : VV0512WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK214

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
Data File : VV025878.D
Acq On : 12 May 2022 13:21
Operator : SY/MD
Sample : VV0512WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK214

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------