

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
 Data File : VV025881.D
 Acq On : 12 May 2022 14:45
 Operator : SY/MD
 Sample : N2714-05ME
 Misc : 5.49g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW2X6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

Signal : TIC: VV025881.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	97	rVB	237060	240553	17.10%	2.288%
2	1.568	157	164	179	rBV	204594	231144	16.43%	2.199%
3	2.108	322	332	353	rVB	431073	619678	44.06%	5.895%
4	2.478	445	447	448	rBV	420	171	0.01%	0.002%
5	2.506	448	456	468	rVV3	5463	9375	0.67%	0.089%
6	2.568	472	475	478	rBV	278	193	0.01%	0.002%
7	2.616	483	490	492	rBV4	940	1139	0.08%	0.011%
8	2.677	508	509	512	rBV2	371	178	0.01%	0.002%
9	2.715	519	521	525	rBV3	317	189	0.01%	0.002%
10	2.735	525	527	530	rVB2	316	140	0.01%	0.001%
11	2.793	543	545	550	rVB2	496	283	0.02%	0.003%
12	2.818	550	553	555	rBV2	275	202	0.01%	0.002%
13	2.841	557	560	563	rBV2	355	285	0.02%	0.003%
14	2.873	568	570	573	rVV	429	260	0.02%	0.002%
15	2.889	573	575	584	rVB3	385	287	0.02%	0.003%
16	3.047	620	624	628	rBV5	628	500	0.04%	0.005%
17	3.066	628	630	634	rVB	352	194	0.01%	0.002%
18	3.095	637	639	643	rVB	480	241	0.02%	0.002%
19	3.137	650	652	653	rBV	342	145	0.01%	0.001%
20	3.182	664	666	669	rBV	260	172	0.01%	0.002%
21	3.243	682	685	687	rBV2	248	147	0.01%	0.001%
22	3.272	693	694	697	rBV	239	125	0.01%	0.001%
23	3.285	697	698	704	rVB2	342	180	0.01%	0.002%
24	3.342	712	716	717	rBV2	270	205	0.01%	0.002%
25	3.391	727	731	734	rBV2	319	211	0.02%	0.002%
26	3.484	757	760	763	rBV	316	192	0.01%	0.002%
27	3.503	763	766	770	rBV3	388	302	0.02%	0.003%
28	3.587	788	792	795	rBV	218	164	0.01%	0.002%
29	3.645	806	810	813	rVV2	341	270	0.02%	0.003%
30	3.661	813	815	821	rBV2	371	320	0.02%	0.003%
31	3.693	821	825	827	rVV2	234	180	0.01%	0.002%
32	3.709	827	830	832	rVV	267	140	0.01%	0.001%
33	3.783	848	853	856	rBV2	405	287	0.02%	0.003%
34	3.905	875	891	931	rBV	61877	279811	19.89%	2.662%
35	4.346	1014	1028	1060	rVB	224166	561949	39.95%	5.346%
36	4.555	1091	1093	1094	rBV	504	165	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW051222\
 Data File : VW025881.D
 Acq On : 12 May 2022 14:45
 Operator : SY/MD
 Sample : N2714-05ME
 Misc : 5.49g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW2X6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

37	4.735	1146	1149	1153	rBV3	361	263	0.02%	0.003%
38	4.786	1163	1165	1168	rVB2	448	190	0.01%	0.002%
39	4.947	1213	1215	1217	rBV2	298	162	0.01%	0.002%
40	5.043	1229	1245	1280	rBV2	546811	1406600	100.00%	13.382%
41	5.497	1384	1386	1389	rBV2	346	228	0.02%	0.002%
42	5.616	1411	1423	1456	rVV	378774	769584	54.71%	7.321%
43	5.828	1487	1489	1493	rVB3	702	451	0.03%	0.004%
44	5.847	1493	1495	1497	rBV2	418	225	0.02%	0.002%
45	5.905	1503	1513	1531	rBV3	15675	34136	2.43%	0.325%
46	6.066	1550	1563	1597	rBV	315481	649917	46.20%	6.183%
47	6.346	1648	1650	1652	rBV2	552	281	0.02%	0.003%
48	6.429	1673	1676	1678	rBV	385	209	0.01%	0.002%
49	6.484	1689	1693	1701	rVB3	512	620	0.04%	0.006%
50	6.548	1710	1713	1715	rBV2	378	217	0.02%	0.002%
51	6.583	1722	1724	1726	rBV	370	206	0.01%	0.002%
52	6.635	1739	1740	1742	rBV	285	144	0.01%	0.001%
53	6.645	1742	1743	1745	rVV	429	132	0.01%	0.001%
54	6.670	1747	1751	1756	rVV5	459	522	0.04%	0.005%
55	6.722	1764	1767	1773	rVB2	307	252	0.02%	0.002%
56	6.747	1773	1775	1777	rBV2	283	173	0.01%	0.002%
57	6.760	1777	1779	1781	rBV2	280	168	0.01%	0.002%
58	6.815	1793	1796	1799	rVB2	400	291	0.02%	0.003%
59	6.841	1802	1804	1807	rVB2	363	166	0.01%	0.002%
60	6.873	1811	1814	1819	rBV2	182	204	0.01%	0.002%
61	6.902	1821	1823	1825	rBV3	373	143	0.01%	0.001%
62	6.985	1834	1849	1882	rBV	154092	296254	21.06%	2.818%
63	7.313	1938	1951	1970	rBV	630508	1076598	76.54%	10.242%
64	7.619	2037	2046	2069	rBV	107534	193790	13.78%	1.844%
65	7.934	2141	2144	2148	rVB3	343	260	0.02%	0.002%
66	7.982	2157	2159	2162	rVB	509	187	0.01%	0.002%
67	8.088	2182	2192	2226	rBV	298358	620637	44.12%	5.904%
68	8.551	2334	2336	2339	rVB	370	166	0.01%	0.002%
69	8.744	2393	2396	2398	rBV2	243	126	0.01%	0.001%
70	8.850	2418	2429	2453	rBV	602712	975561	69.36%	9.281%
71	9.146	2516	2521	2524	rBV4	912	970	0.07%	0.009%
72	9.384	2591	2595	2600	rBV2	332	265	0.02%	0.003%
73	9.413	2602	2604	2608	rVV2	344	176	0.01%	0.002%
74	9.432	2608	2610	2613	rVB	399	185	0.01%	0.002%
75	9.587	2656	2658	2659	rBV	450	168	0.01%	0.002%
76	9.741	2704	2706	2708	rBV	287	138	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW051222\
 Data File : VW025881.D
 Acq On : 12 May 2022 14:45
 Operator : SY/MD
 Sample : N2714-05ME
 Misc : 5.49g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW2X6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

77	9.780	2716	2718	2721	rBV2	361	189	0.01%	0.002%
78	9.879	2747	2749	2752	rVB	334	142	0.01%	0.001%
79	9.956	2770	2773	2777	rBV2	325	247	0.02%	0.002%
80	9.995	2783	2785	2787	rBV	366	128	0.01%	0.001%
81	10.124	2818	2825	2835	rVB3	2544	3883	0.28%	0.037%
82	10.214	2839	2853	2874	rBV	411231	649218	46.16%	6.176%
83	10.374	2901	2903	2904	rBV	592	280	0.02%	0.003%
84	10.426	2917	2919	2923	rBV	243	172	0.01%	0.002%
85	10.448	2923	2926	2928	rBV2	387	211	0.02%	0.002%
86	10.490	2936	2939	2941	rBV2	449	272	0.02%	0.003%
87	10.532	2950	2952	2953	rBV	321	136	0.01%	0.001%
88	10.693	2997	3002	3005	rBV2	295	337	0.02%	0.003%
89	10.767	3023	3025	3027	rBV	302	156	0.01%	0.001%
90	10.841	3045	3048	3052	rVB3	809	592	0.04%	0.006%
91	10.918	3062	3072	3076	rBV8	1808	2686	0.19%	0.026%
92	11.062	3115	3117	3119	rVB	435	139	0.01%	0.001%
93	11.146	3138	3143	3147	rBV4	1304	1363	0.10%	0.013%
94	11.197	3153	3159	3162	rBV2	486	412	0.03%	0.004%
95	11.246	3162	3174	3207	rVV	589061	905593	64.38%	8.615%
96	11.622	3278	3291	3315	rBV	615803	963437	68.49%	9.166%
97	12.802	3656	3658	3661	rBV	339	205	0.01%	0.002%
98	12.914	3691	3693	3694	rBV	457	206	0.01%	0.002%
99	13.799	3964	3968	3970	rBV2	492	335	0.02%	0.003%
100	13.895	3996	3998	4000	rBV	407	191	0.01%	0.002%


Sum of corrected areas: 10511472

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
Data File : VV025881.D
Acq On : 12 May 2022 14:45
Operator : SY/MD
Sample : N2714-05ME
Misc : 5.49g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW2X6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

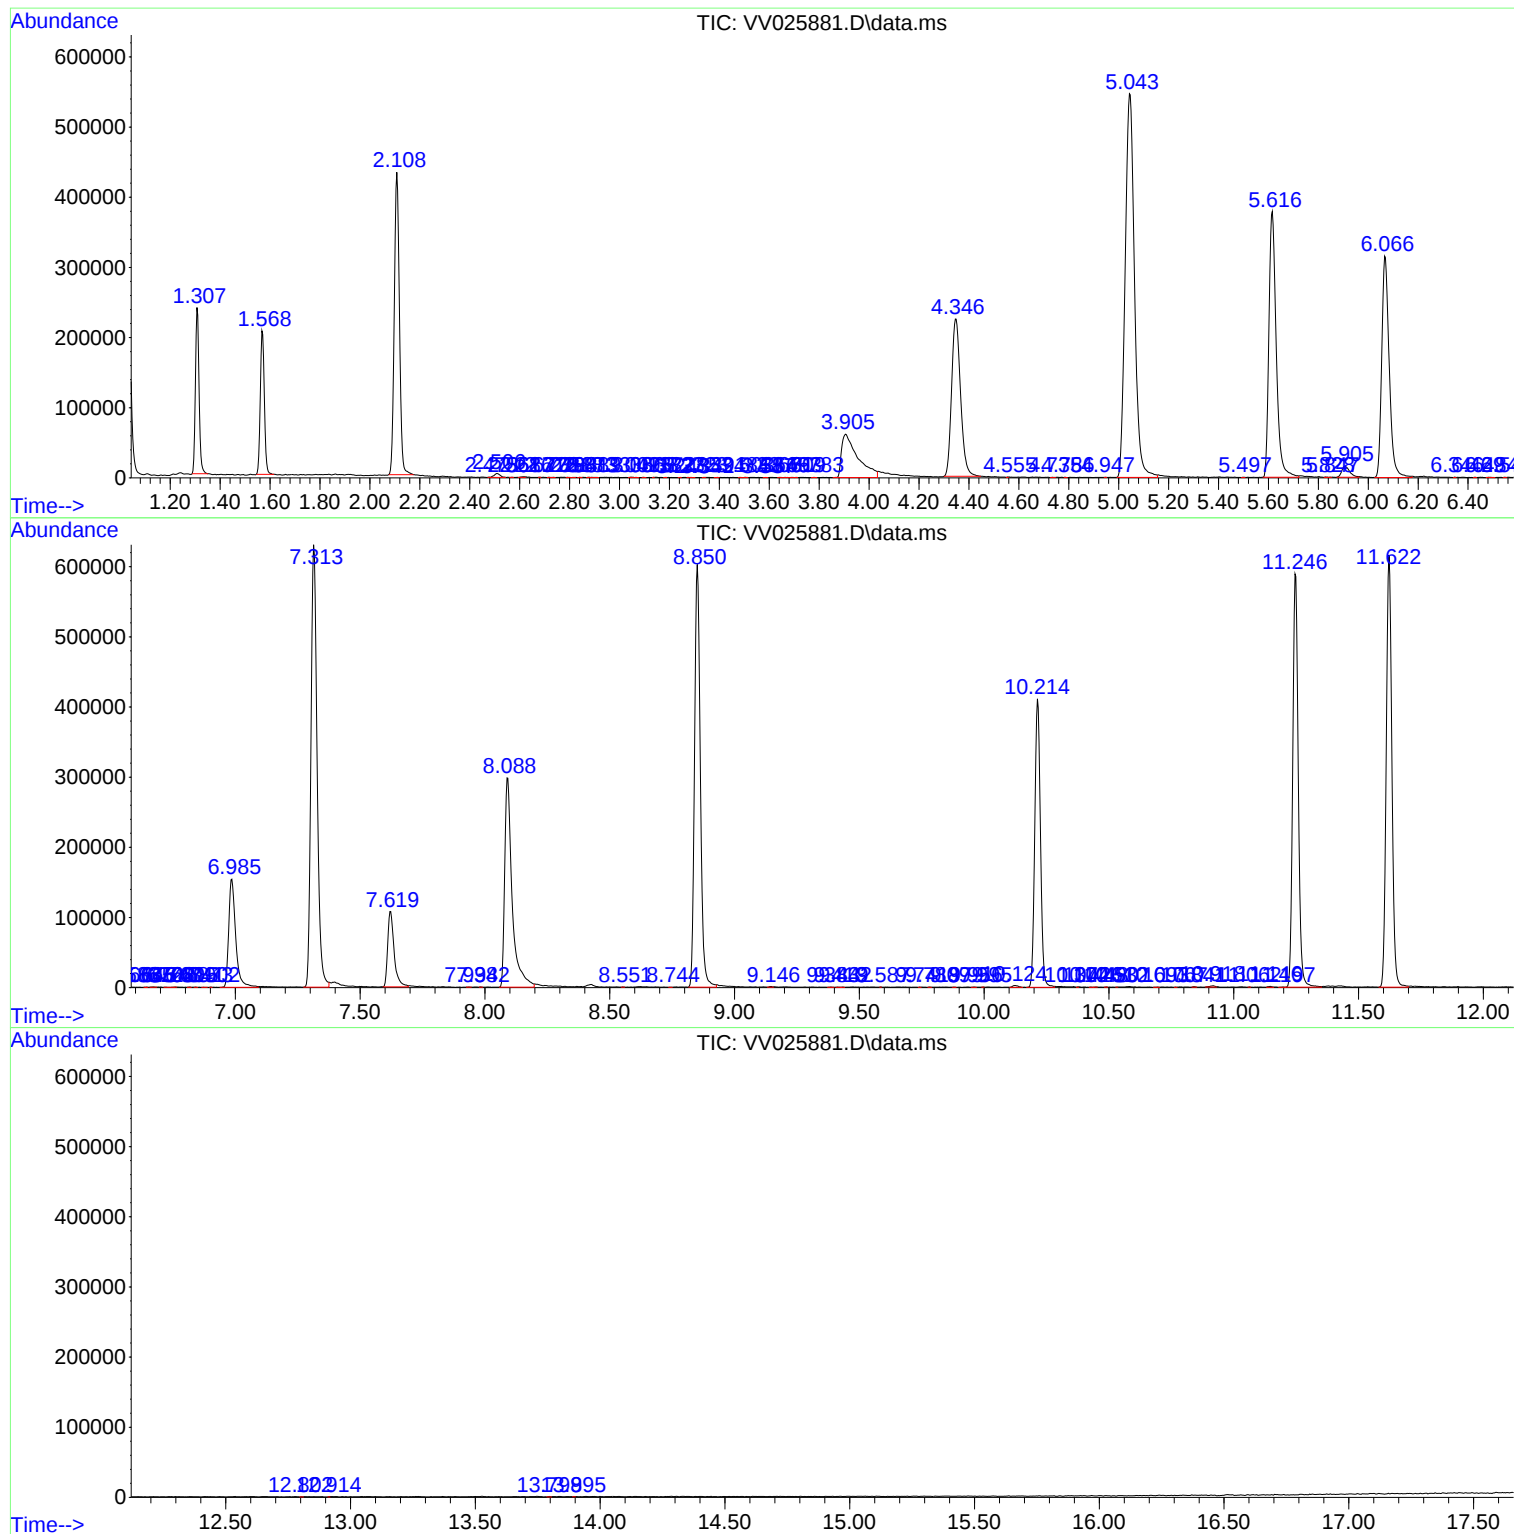

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
Data File : VV025881.D
Acq On : 12 May 2022 14:45
Operator : SY/MD
Sample : N2714-05ME
Misc : 5.49g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW2X6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
Data File : VV025881.D
Acq On : 12 May 2022 14:45
Operator : SY/MD
Sample : N2714-05ME
Misc : 5.49g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW2X6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc