

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
 Data File : VV025885.D
 Acq On : 12 May 2022 16:20
 Operator : SY/MD
 Sample : N2713-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBSK9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

Signal : TIC: VV025885.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	97	rVB	236791	245104	17.39%	2.385%
2	1.571	157	165	181	rVB	208792	236718	16.79%	2.303%
3	2.108	322	332	365	rVB	435207	631219	44.78%	6.141%
4	2.433	431	433	435	rBV2	480	209	0.01%	0.002%
5	2.574	474	477	479	rBV2	353	222	0.02%	0.002%
6	2.719	520	522	525	rVB2	540	254	0.02%	0.002%
7	2.757	532	534	540	rVB2	438	323	0.02%	0.003%
8	2.796	544	546	549	rBV2	351	192	0.01%	0.002%
9	2.834	556	558	562	rBV2	274	157	0.01%	0.002%
10	3.056	624	627	633	rVB4	435	383	0.03%	0.004%
11	3.085	633	636	637	rBV4	441	214	0.02%	0.002%
12	3.121	642	647	650	rVV2	616	472	0.03%	0.005%
13	3.185	663	667	670	rBV2	295	199	0.01%	0.002%
14	3.211	670	675	679	rVB3	288	244	0.02%	0.002%
15	3.285	696	698	703	rVV3	293	266	0.02%	0.003%
16	3.474	754	757	763	rBV2	294	248	0.02%	0.002%
17	3.503	763	766	770	rVB2	381	245	0.02%	0.002%
18	3.613	798	800	802	rBV	362	179	0.01%	0.002%
19	3.658	812	814	815	rBV	321	154	0.01%	0.001%
20	3.677	818	820	827	rVB	267	197	0.01%	0.002%
21	3.744	839	841	845	rBV2	245	169	0.01%	0.002%
22	3.780	849	852	858	rVB2	353	223	0.02%	0.002%
23	3.905	881	891	931	rBV2	62631	275357	19.53%	2.679%
24	4.349	1015	1029	1063	rVB	224666	559726	39.71%	5.446%
25	4.648	1120	1122	1124	rBV	474	262	0.02%	0.003%
26	4.703	1137	1139	1142	rBV2	311	193	0.01%	0.002%
27	4.722	1142	1145	1149	rVV3	482	422	0.03%	0.004%
28	4.831	1177	1179	1181	rBV	291	167	0.01%	0.002%
29	4.844	1181	1183	1186	rVV	462	263	0.02%	0.003%
30	4.879	1189	1194	1195	rBV	369	270	0.02%	0.003%
31	4.915	1200	1205	1208	rVV3	619	481	0.03%	0.005%
32	4.944	1212	1214	1218	rBV4	355	230	0.02%	0.002%
33	5.047	1229	1246	1281	rBV2	546232	1409709	100.00%	13.716%
34	5.352	1337	1341	1344	rBV2	530	421	0.03%	0.004%
35	5.378	1346	1349	1354	rVB3	632	526	0.04%	0.005%
36	5.410	1357	1359	1361	rBV3	440	265	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW051222\
 Data File : VW025885.D
 Acq On : 12 May 2022 16:20
 Operator : SY/MD
 Sample : N2713-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBSK9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

37	5.519	1391	1393	1395	rBV3	410	189	0.01%	0.002%
38	5.616	1412	1423	1454	rBV	344306	707588	50.19%	6.884%
39	5.905	1504	1513	1529	rBV2	15701	34088	2.42%	0.332%
40	6.069	1546	1564	1597	rBV	316600	657607	46.65%	6.398%
41	6.326	1643	1644	1647	rVB	582	205	0.01%	0.002%
42	6.387	1661	1663	1665	rBV2	309	153	0.01%	0.001%
43	6.416	1668	1672	1676	rVV3	659	598	0.04%	0.006%
44	6.436	1676	1678	1683	rVV2	430	417	0.03%	0.004%
45	6.481	1690	1692	1695	rVB2	359	171	0.01%	0.002%
46	6.516	1700	1703	1707	rVB2	397	349	0.02%	0.003%
47	6.542	1707	1711	1713	rBV	286	241	0.02%	0.002%
48	6.619	1732	1735	1736	rBV	314	182	0.01%	0.002%
49	6.664	1747	1749	1752	rBV	323	177	0.01%	0.002%
50	6.719	1763	1766	1769	rBV3	480	288	0.02%	0.003%
51	6.764	1774	1780	1784	rBV3	295	392	0.03%	0.004%
52	6.786	1784	1787	1789	rBV	302	158	0.01%	0.002%
53	6.870	1810	1813	1814	rBV	330	192	0.01%	0.002%
54	6.908	1822	1825	1828	rBV2	269	208	0.01%	0.002%
55	6.937	1832	1834	1838	rVB2	423	218	0.02%	0.002%
56	6.985	1838	1849	1881	rBV	153157	287426	20.39%	2.796%
57	7.317	1940	1952	1973	rBV	613680	1070532	75.94%	10.416%
58	7.622	2036	2047	2074	rBV	108675	195468	13.87%	1.902%
59	7.796	2098	2101	2102	rBV2	662	387	0.03%	0.004%
60	7.895	2128	2132	2135	rBV3	520	377	0.03%	0.004%
61	7.918	2135	2139	2140	rBV2	323	207	0.01%	0.002%
62	7.982	2155	2159	2161	rBV3	555	377	0.03%	0.004%
63	8.014	2165	2169	2171	rVB3	423	288	0.02%	0.003%
64	8.043	2175	2178	2180	rBV3	278	167	0.01%	0.002%
65	8.091	2183	2193	2223	rBV	313970	638254	45.28%	6.210%
66	8.510	2321	2323	2327	rBV3	528	324	0.02%	0.003%
67	8.715	2385	2387	2389	rVV	396	154	0.01%	0.001%
68	8.767	2399	2403	2407	rVB4	469	380	0.03%	0.004%
69	8.850	2415	2429	2452	rBV	552963	903526	64.09%	8.791%
70	9.252	2550	2554	2556	rBV2	338	207	0.01%	0.002%
71	9.288	2562	2565	2566	rBV2	278	159	0.01%	0.002%
72	9.329	2575	2578	2581	rBV2	341	261	0.02%	0.003%
73	9.426	2604	2608	2611	rVB2	361	269	0.02%	0.003%
74	9.603	2661	2663	2668	rVB2	297	187	0.01%	0.002%
75	9.728	2699	2702	2704	rBV2	268	200	0.01%	0.002%
76	9.757	2708	2711	2716	rVB2	394	305	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
 Data File : VV025885.D
 Acq On : 12 May 2022 16:20
 Operator : SY/MD
 Sample : N2713-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBSK9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

77	9.783	2716	2719	2721	rBV2	376	257	0.02%	0.003%
78	10.008	2784	2789	2792	rVB	334	239	0.02%	0.002%
79	10.072	2804	2809	2810	rBV2	380	293	0.02%	0.003%
80	10.130	2818	2827	2832	rBV5	1891	2845	0.20%	0.028%
81	10.175	2838	2841	2842	rBV2	527	276	0.02%	0.003%
82	10.214	2842	2853	2874	rVV	416640	649649	46.08%	6.321%
83	10.506	2941	2944	2945	rBV	331	202	0.01%	0.002%
84	10.535	2950	2953	2954	rBV	356	196	0.01%	0.002%
85	10.571	2960	2964	2968	rBV5	587	509	0.04%	0.005%
86	10.596	2968	2972	2974	rVV3	456	303	0.02%	0.003%
87	10.657	2987	2991	2994	rBV3	622	458	0.03%	0.004%
88	10.728	3011	3013	3016	rVB	313	179	0.01%	0.002%
89	10.744	3016	3018	3021	rBV2	358	278	0.02%	0.003%
90	10.799	3031	3035	3041	rBV2	701	971	0.07%	0.009%
91	10.879	3058	3060	3062	rBV2	349	178	0.01%	0.002%
92	11.101	3124	3129	3130	rBV2	352	249	0.02%	0.002%
93	11.140	3138	3141	3143	rBV2	1403	918	0.07%	0.009%
94	11.249	3163	3175	3199	rBV	517655	813005	57.67%	7.910%
95	11.622	3279	3291	3311	rBV	601600	936061	66.40%	9.107%
96	11.866	3366	3367	3371	rBV	383	195	0.01%	0.002%
97	12.001	3405	3409	3411	rBV	495	347	0.02%	0.003%
98	12.535	3569	3575	3580	rBV5	634	884	0.06%	0.009%
99	14.500	4183	4186	4189	rBV2	510	439	0.03%	0.004%
100	14.741	4259	4261	4265	rBV2	567	412	0.03%	0.004%




Sum of corrected areas: 10278102

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
Data File : VV025885.D
Acq On : 12 May 2022 16:20
Operator : SY/MD
Sample : N2713-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBSK9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

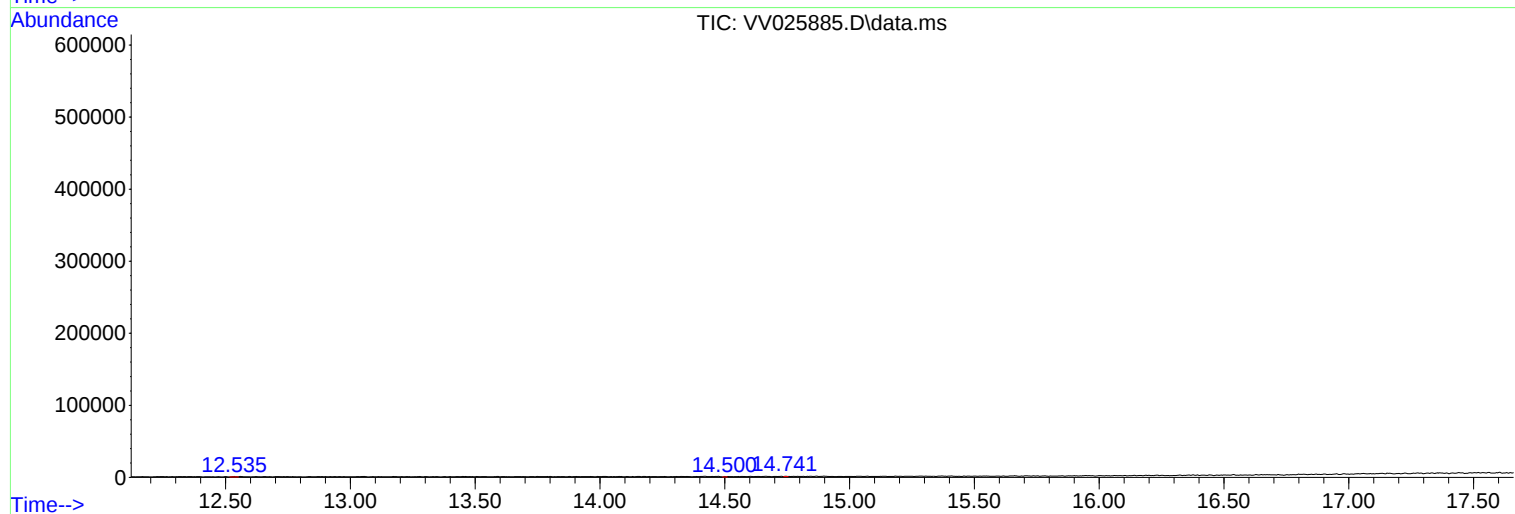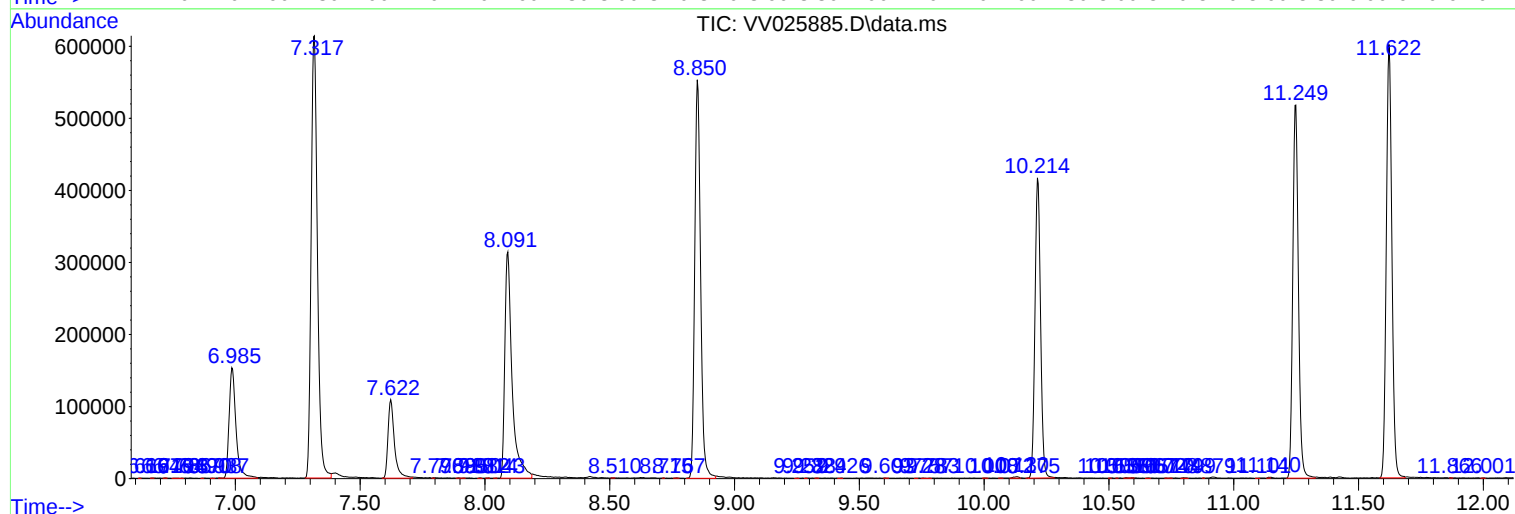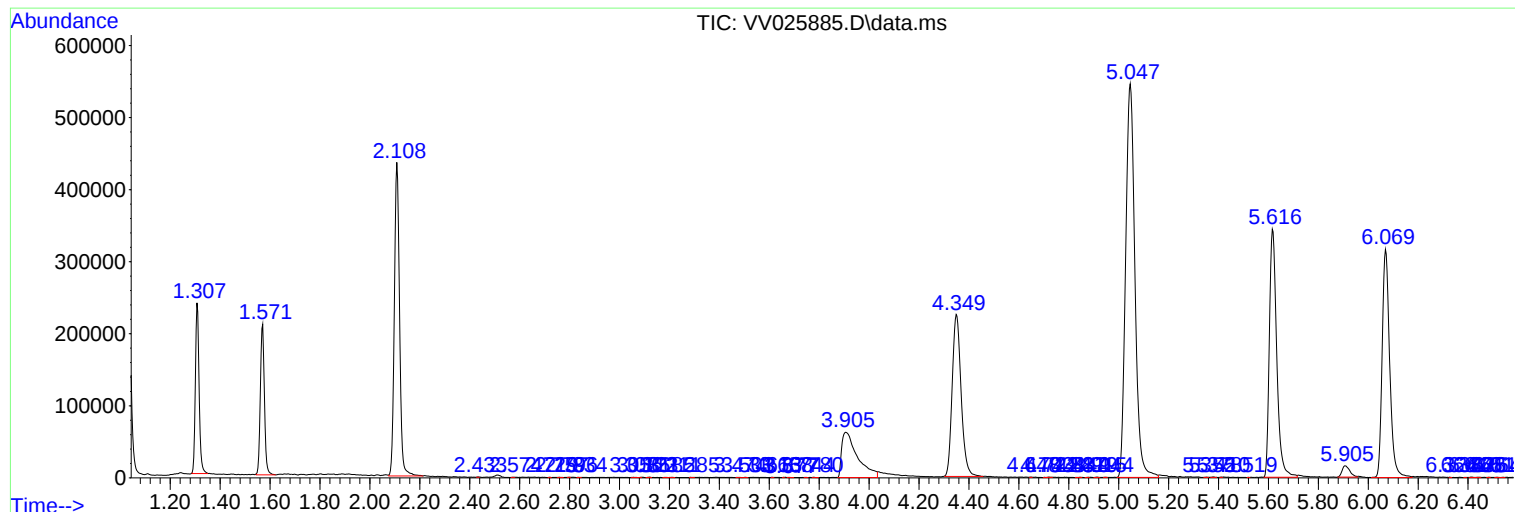

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
Data File : VV025885.D
Acq On : 12 May 2022 16:20
Operator : SY/MD
Sample : N2713-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBSK9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
Data File : VV025885.D
Acq On : 12 May 2022 16:20
Operator : SY/MD
Sample : N2713-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBSK9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------