

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
 Data File : VV025886.D
 Acq On : 12 May 2022 16:44
 Operator : SY/MD
 Sample : N2713-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBSL5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

Signal : TIC: VV025886.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	99	rVB	224113	231926	17.01%	2.336%
2	1.568	157	164	178	rVB	197053	224660	16.48%	2.263%
3	2.108	323	332	360	rVB	415307	601259	44.10%	6.056%
4	2.506	451	456	465	rVB5	3128	4643	0.34%	0.047%
5	2.596	481	484	487	rBV3	357	226	0.02%	0.002%
6	2.619	487	491	496	rBV3	632	654	0.05%	0.007%
7	2.728	522	525	527	rBV2	373	246	0.02%	0.002%
8	2.767	534	537	538	rBV3	268	163	0.01%	0.002%
9	2.777	538	540	542	rVB	385	170	0.01%	0.002%
10	2.847	560	562	566	rVB2	426	234	0.02%	0.002%
11	2.873	567	570	578	rVB	453	422	0.03%	0.004%
12	2.905	578	580	584	rBV	322	303	0.02%	0.003%
13	2.976	599	602	603	rBV	505	195	0.01%	0.002%
14	2.989	603	606	608	rBV2	275	152	0.01%	0.002%
15	3.230	675	681	686	rBV2	520	647	0.05%	0.007%
16	3.375	724	726	727	rBV2	343	140	0.01%	0.001%
17	3.429	739	743	745	rBV	324	210	0.02%	0.002%
18	3.555	778	782	784	rBV	410	241	0.02%	0.002%
19	3.770	847	849	855	rBV2	228	135	0.01%	0.001%
20	3.805	856	860	863	rBV3	273	180	0.01%	0.002%
21	3.908	881	892	935	rBV2	62102	277987	20.39%	2.800%
22	4.349	1015	1029	1054	rBV	218928	534612	39.21%	5.385%
23	4.555	1088	1093	1096	rBV5	734	558	0.04%	0.006%
24	4.715	1141	1143	1146	rVB2	430	238	0.02%	0.002%
25	4.738	1146	1150	1154	rBV3	528	544	0.04%	0.005%
26	4.854	1184	1186	1190	rBV3	270	137	0.01%	0.001%
27	4.889	1190	1197	1200	rBV4	463	534	0.04%	0.005%
28	4.937	1210	1212	1217	rBV3	263	235	0.02%	0.002%
29	5.047	1229	1246	1288	rVV2	529737	1363502	100.00%	13.733%
30	5.484	1379	1382	1384	rBV3	809	507	0.04%	0.005%
31	5.555	1400	1404	1405	rBV2	370	223	0.02%	0.002%
32	5.616	1412	1423	1453	rBV	329457	672264	49.30%	6.771%
33	5.908	1505	1514	1536	rVV2	15533	33543	2.46%	0.338%
34	6.069	1551	1564	1588	rBV	303089	625258	45.86%	6.298%
35	6.333	1644	1646	1648	rBV	277	145	0.01%	0.001%
36	6.349	1649	1651	1653	rVV2	451	255	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
 Data File : VV025886.D
 Acq On : 12 May 2022 16:44
 Operator : SY/MD
 Sample : N2713-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBSL5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

37	6.358	1653	1654	1659	rVB3	777	406	0.03%	0.004%
38	6.400	1664	1667	1669	rBV2	522	229	0.02%	0.002%
39	6.471	1688	1689	1695	rVB2	370	196	0.01%	0.002%
40	6.503	1695	1699	1701	rBV2	429	203	0.01%	0.002%
41	6.593	1723	1727	1728	rBV	281	165	0.01%	0.002%
42	6.625	1735	1737	1741	rBV2	325	200	0.01%	0.002%
43	6.645	1741	1743	1746	rVV2	342	181	0.01%	0.002%
44	6.664	1746	1749	1753	rVB3	381	268	0.02%	0.003%
45	6.683	1753	1755	1756	rBV	337	168	0.01%	0.002%
46	6.693	1756	1758	1762	rVB2	552	303	0.02%	0.003%
47	6.715	1762	1765	1767	rBV2	546	302	0.02%	0.003%
48	6.728	1767	1769	1772	rVV2	416	219	0.02%	0.002%
49	6.760	1776	1779	1781	rBV2	295	167	0.01%	0.002%
50	6.892	1818	1820	1830	rVB3	420	471	0.03%	0.005%
51	6.931	1830	1832	1836	rBV	282	210	0.02%	0.002%
52	6.985	1837	1849	1877	rBV	148767	279280	20.48%	2.813%
53	7.317	1940	1952	1971	rBV	585153	1022086	74.96%	10.294%
54	7.622	2037	2047	2069	rBV	103815	186251	13.66%	1.876%
55	7.837	2112	2114	2116	rBV3	673	311	0.02%	0.003%
56	7.882	2125	2128	2129	rBV3	465	260	0.02%	0.003%
57	7.969	2152	2155	2156	rBV2	359	199	0.01%	0.002%
58	8.008	2164	2167	2170	rBV	277	168	0.01%	0.002%
59	8.091	2181	2193	2239	rBV	315557	644806	47.29%	6.494%
60	8.419	2288	2295	2309	rBV6	2474	4386	0.32%	0.044%
61	8.590	2344	2348	2350	rBV2	384	325	0.02%	0.003%
62	8.699	2379	2382	2383	rBV	309	173	0.01%	0.002%
63	8.734	2390	2393	2394	rBV2	339	211	0.02%	0.002%
64	8.850	2418	2429	2463	rVV	529200	867901	63.65%	8.741%
65	9.156	2522	2524	2527	rVB4	790	384	0.03%	0.004%
66	9.239	2548	2550	2552	rVB	503	182	0.01%	0.002%
67	9.259	2552	2556	2557	rBV	310	195	0.01%	0.002%
68	9.381	2591	2594	2597	rBV2	294	164	0.01%	0.002%
69	9.490	2625	2628	2632	rVB3	331	221	0.02%	0.002%
70	9.583	2654	2657	2660	rBV2	331	239	0.02%	0.002%
71	9.648	2675	2677	2681	rBV	574	277	0.02%	0.003%
72	9.763	2711	2713	2717	rVB	479	227	0.02%	0.002%
73	9.805	2724	2726	2730	rVB	402	215	0.02%	0.002%
74	9.828	2730	2733	2735	rBV	276	142	0.01%	0.001%
75	9.844	2735	2738	2740	rVB	369	135	0.01%	0.001%
76	9.863	2741	2744	2748	rBV2	265	209	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
 Data File : VV025886.D
 Acq On : 12 May 2022 16:44
 Operator : SY/MD
 Sample : N2713-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBSL5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

77	9.886	2748	2751	2752	rBV2	258	174	0.01%	0.002%
78	10.017	2790	2792	2794	rBV	370	163	0.01%	0.002%
79	10.075	2807	2810	2817	rBV	287	271	0.02%	0.003%
80	10.130	2817	2827	2834	rVB5	2221	3487	0.26%	0.035%
81	10.214	2841	2853	2875	rBV	409781	644274	47.25%	6.489%
82	10.355	2895	2897	2902	rBV4	591	570	0.04%	0.006%
83	10.442	2922	2924	2928	rVB2	311	210	0.02%	0.002%
84	10.522	2947	2949	2952	rVB2	423	168	0.01%	0.002%
85	10.545	2952	2956	2959	rBV2	352	345	0.03%	0.003%
86	10.654	2987	2990	2991	rBV2	300	141	0.01%	0.001%
87	10.760	3021	3023	3025	rBV2	436	174	0.01%	0.002%
88	10.789	3029	3032	3035	rBV2	393	306	0.02%	0.003%
89	10.828	3042	3044	3046	rVB	479	191	0.01%	0.002%
90	10.918	3064	3072	3076	rBV6	1268	1983	0.15%	0.020%
91	11.078	3119	3122	3125	rBV2	377	190	0.01%	0.002%
92	11.178	3150	3153	3155	rBV3	508	265	0.02%	0.003%
93	11.249	3164	3175	3205	rBV	503378	782292	57.37%	7.879%
94	11.464	3240	3242	3243	rBV	360	140	0.01%	0.001%
95	11.622	3278	3291	3311	rBV	567246	901320	66.10%	9.078%
96	12.075	3429	3432	3433	rBV2	392	250	0.02%	0.003%
97	12.789	3649	3654	3659	rBV2	544	598	0.04%	0.006%
98	12.911	3689	3692	3696	rVB3	666	475	0.03%	0.005%
99	13.049	3732	3735	3741	rBV2	649	423	0.03%	0.004%
100	13.120	3755	3757	3759	rBV2	429	219	0.02%	0.002%


Sum of corrected areas: 9928612

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
Data File : VV025886.D
Acq On : 12 May 2022 16:44
Operator : SY/MD
Sample : N2713-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBSL5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

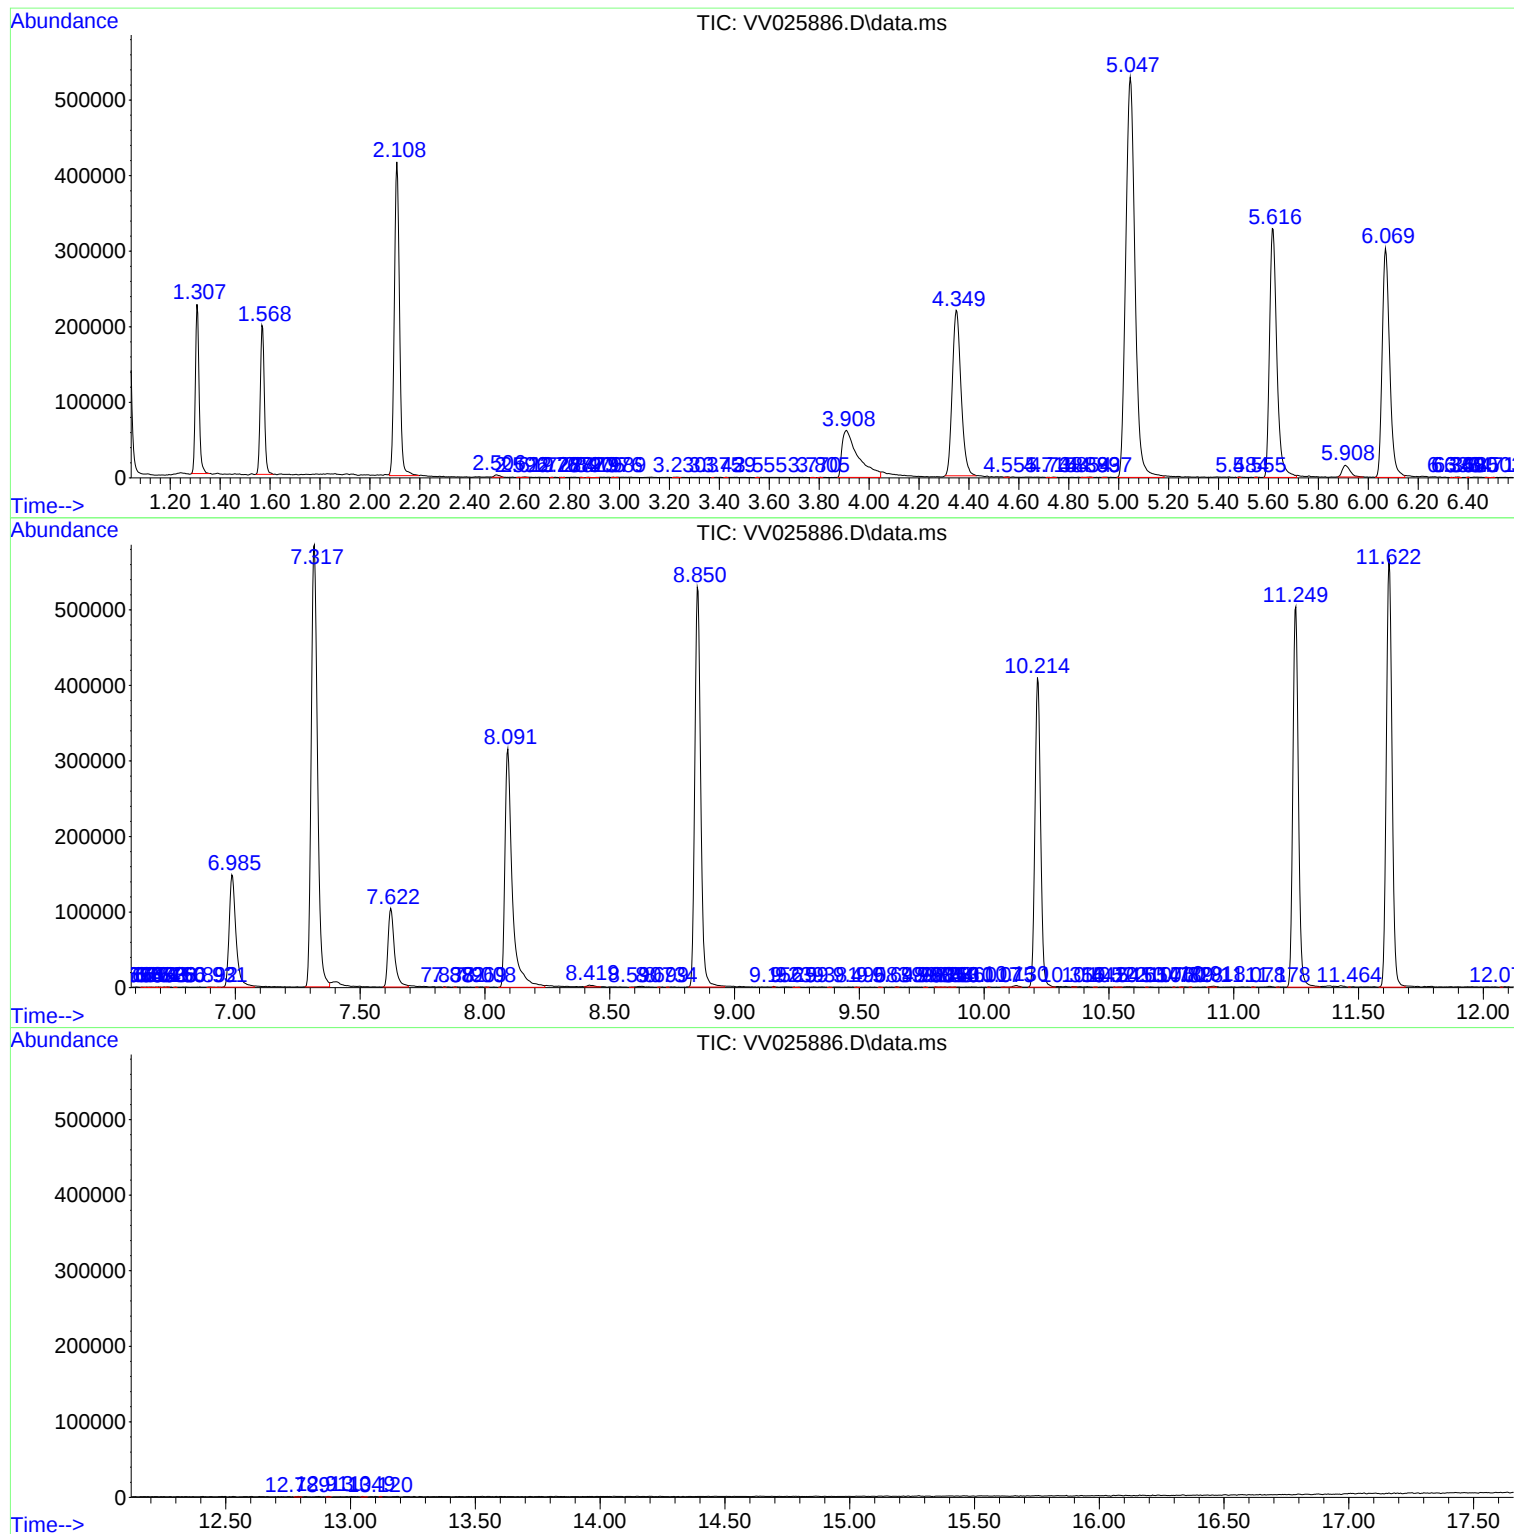

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
Data File : VV025886.D
Acq On : 12 May 2022 16:44
Operator : SY/MD
Sample : N2713-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBSL5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
Data File : VV025886.D
Acq On : 12 May 2022 16:44
Operator : SY/MD
Sample : N2713-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBSL5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
