
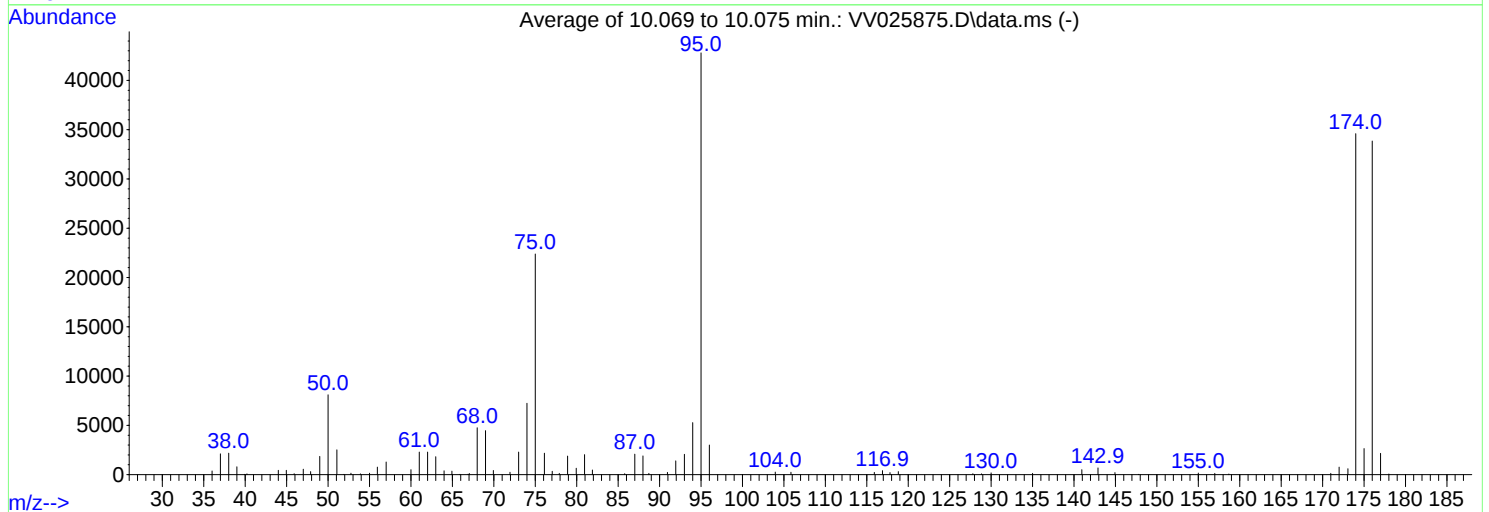


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051222\
 Data File : VV025875.D
 Acq On : 12 May 2022 11:23
 Operator : SY/MD
 Sample : BFB282
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB282

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis
 Last Update : Fri May 13 07:07:32 2022

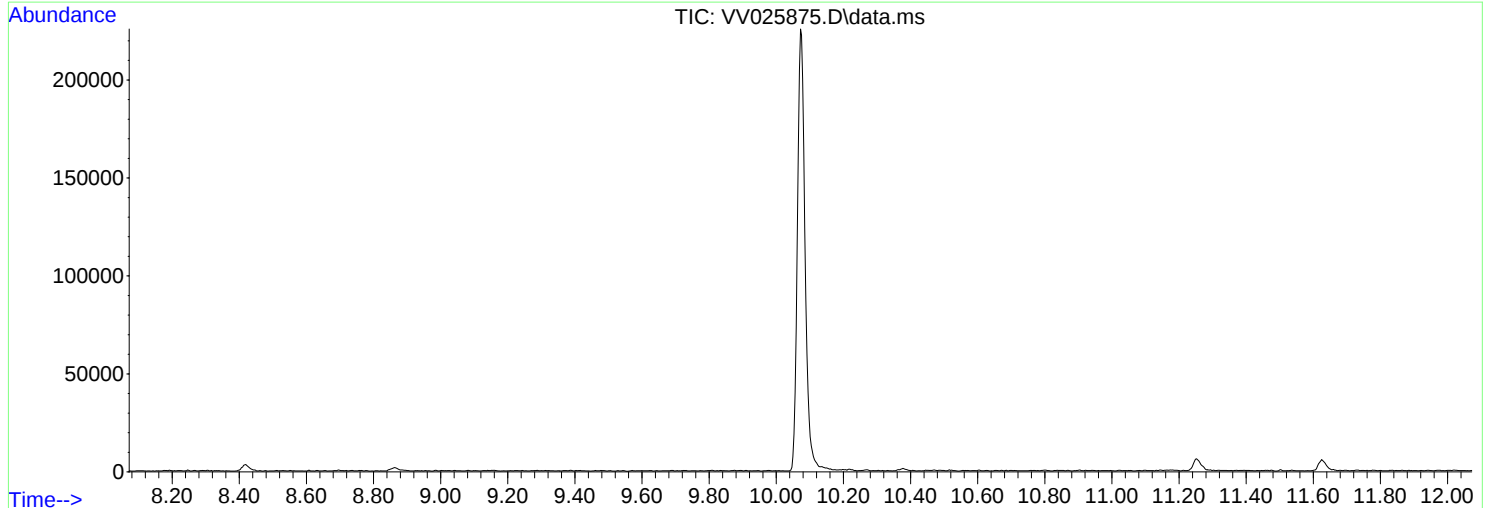

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	8106	PASS
75	95	30	80	52.3	22392	PASS
95	95	100	100	100.0	42795	PASS
96	95	5	9	7.0	3006	PASS
173	174	0.00	2	1.7	600	PASS
174	95	50	120	80.8	34592	PASS
175	174	5	9	7.6	2645	PASS
176	174	95	105	97.8	33840	PASS
177	176	5	10	6.4	2152	PASS

m/z	Abundance
40.00	208.0
44.10	286.0

Instrument :
MSVOA_V
ClientSampleId :
BFB282

m/z	Abundance
36.00	345.0
37.00	2090.0
38.00	2063.0
39.00	864.0
39.90	223.0
40.20	234.0
44.00	693.0
45.00	418.0
45.90	151.0
46.90	506.0
47.90	325.0
49.00	1841.0
50.00	7767.0
51.00	2418.0
52.80	154.0
55.00	165.0
55.90	726.0
57.00	1305.0
60.00	485.0
61.00	2068.0
62.00	2203.0
63.00	1701.0
64.00	328.0
65.00	325.0
66.90	137.0
68.00	4496.0
69.00	4211.0
69.90	437.0
71.90	251.0
73.00	2214.0
74.00	6845.0
75.00	21568.0
76.10	2018.0
77.10	348.0
78.90	1812.0
80.00	616.0
80.90	1957.0
81.90	427.0
87.00	1949.0
88.00	1786.0
88.70	178.0
90.90	195.0
92.00	1283.0
93.00	1907.0
94.00	4980.0
95.00	40024.0
96.00	2842.0
104.00	257.0
105.90	229.0
115.90	221.0
116.90	435.0
117.70	199.0
118.80	325.0
130.00	167.0
135.00	126.0
141.00	462.0
142.90	618.0
145.00	180.0
147.80	100.0
155.00	111.0
157.00	121.0
171.00	107.0
172.00	698.0
173.00	498.0
174.00	32480.0
175.00	2467.0
176.00	31192.0
177.00	2027.0

Instrument :
MSVOA_V
ClientSampleId :
BFB282

m/z	Abundance
36.00	389.0
37.00	2187.0
38.00	2238.0
39.00	806.0
39.90	245.0
44.00	755.0
45.00	466.0
45.90	138.0
47.00	578.0
47.90	308.0
49.00	1889.0
50.00	8369.0
51.00	2613.0
52.80	154.0
53.90	112.0
55.00	157.0
56.00	812.0
57.00	1321.0
60.00	526.0
61.00	2370.0
62.00	2410.0
63.00	1894.0
64.00	402.0
65.00	359.0
65.90	120.0
67.10	171.0
68.00	4953.0
69.00	4563.0
70.00	430.0
72.00	246.0
73.00	2361.0
74.00	7475.0
75.00	23208.0
76.10	2264.0
77.10	356.0
77.90	201.0
78.90	1969.0
79.90	657.0
81.00	2080.0
81.90	493.0
85.80	150.0
87.00	2193.0
88.00	1945.0
88.70	231.0
91.00	235.0
92.00	1447.0
93.00	2128.0
94.00	5521.0
95.00	44328.0
96.00	3148.0
104.00	262.0
105.90	254.0
115.90	240.0
116.90	436.0
117.80	200.0
118.80	301.0
127.80	122.0
128.80	101.0
130.00	194.0
135.00	134.0
140.90	532.0
142.90	705.0
144.90	219.0
155.00	184.0
157.00	149.0
158.70	108.0
171.00	134.0
172.00	803.0
173.10	612.0
174.00	35680.0
175.00	2730.0
176.00	35208.0
177.00	2230.0
178.00	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB282

m/z	Abundance
36.00	383.0
37.00	2071.0
38.00	2205.0
39.00	736.0
39.90	247.0
44.00	730.0
44.90	415.0
47.10	585.0
47.90	319.0
49.00	1823.0
50.00	8182.0
51.10	2540.0
51.90	103.0
52.60	120.0
53.90	120.0
55.00	139.0
56.00	757.0
57.00	1207.0
60.00	493.0
61.00	2429.0
62.00	2259.0
63.00	1848.0
64.00	465.0
64.90	399.0
67.00	190.0
68.00	4815.0
69.00	4620.0
70.00	417.0
72.00	249.0
73.00	2274.0
74.00	7391.0
75.00	22400.0
76.10	2231.0
76.90	339.0
77.90	199.0
78.90	1859.0
79.90	679.0
80.90	2068.0
81.90	518.0
85.80	157.0
87.00	2108.0
88.00	1960.0
91.00	264.0
91.90	1469.0
93.00	2136.0
94.00	5344.0
95.00	44032.0
96.00	3029.0
103.90	261.0
105.80	271.0
115.90	199.0
116.90	375.0
117.90	240.0
118.80	289.0
127.80	186.0
128.90	123.0
130.00	192.0
135.00	123.0
140.90	511.0
142.90	745.0
144.90	253.0
155.00	210.0
157.00	148.0
158.70	106.0
171.00	145.0
172.00	769.0
173.10	691.0
174.00	35616.0
175.00	2738.0
176.00	35120.0
177.00	2198.0
178.00	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB282