


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051319\
 Data File : VV010844.D
 Acq On : 13 May 2019 17:15
 Operator : SY/MD
 Sample : BFB63

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB63

Misc : 5.00G/10ML/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM051319S.M
 Title : VOC Analysis
 Last Update : Mon May 13 14:46:08 2019

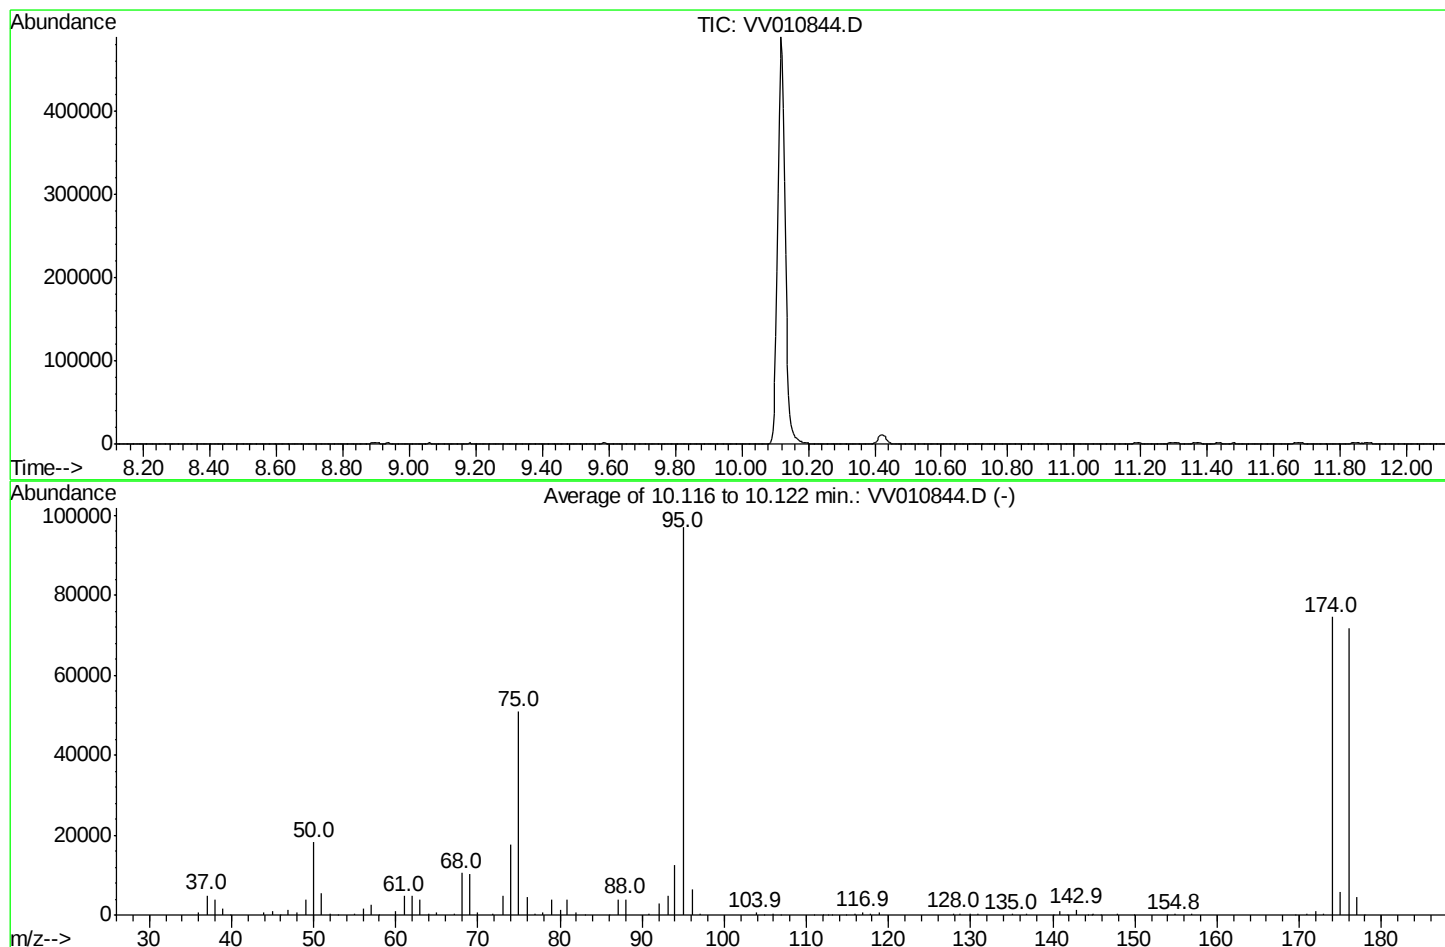

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2795

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.7	18125	PASS
75	95	30	80	52.5	50925	PASS
95	95	100	100	100.0	97034	PASS
96	95	5	9	6.5	6333	PASS
173	174	0.00	2	0.5	362	PASS
174	95	50	120	76.8	74533	PASS
175	174	5	9	7.9	5914	PASS
176	174	95	101	96.3	71805	PASS
177	176	5	9	6.1	4405	PASS

Scan 2795 (10.077 min): VV010844.D
BFB63

m/z	Abundance
39.90	160.0
44.00	184.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
36.00	818.0
37.00	4826.0
38.00	3819.0
39.00	1752.0
39.90	230.0
43.90	731.0
45.00	919.0
46.00	182.0
47.00	1217.0
48.00	528.0
49.00	3900.0
50.00	18208.0
51.00	5291.0
52.00	237.0
52.90	124.0
55.00	334.0
56.00	1553.0
57.00	2809.0
57.90	135.0
60.00	946.0
61.00	4307.0
62.00	4925.0
63.00	3763.0
64.00	519.0
65.00	634.0
67.10	274.0
68.00	10290.0
69.00	9861.0
70.00	781.0
71.90	459.0
73.00	4713.0
74.00	17264.0
75.00	50232.0
76.00	4434.0
77.10	460.0
77.80	496.0
78.90	3700.0
80.00	1226.0
80.90	3865.0
81.90	836.0
82.90	101.0
85.90	169.0
87.00	3851.0
88.00	3775.0
90.90	416.0
92.00	3045.0
93.10	4268.0
94.00	12217.0
95.00	95872.0
96.10	6566.0
97.00	172.0
103.90	518.0
104.80	191.0
105.90	461.0
106.80	146.0
110.90	137.0
112.60	114.0
113.10	141.0
115.90	434.0
116.90	626.0
117.80	387.0
118.90	592.0
128.00	348.0
128.70	166.0
129.90	317.0
130.80	190.0
135.00	223.0
136.90	173.0
140.00	113.0
140.90	1127.0
141.80	151.0
142.90	1299.0
145.00	217.0
145.80	171.0
147.80	306.0
149.90	142.0
153.90	115.0
154.80	221.0
156.90	165.0
170.90	149.0
172.00	961.0
174.00	71416.0
175.00	5679.0
176.00	68536.0
177.00	4464.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
36.00	817.0
37.00	5114.0
38.00	3886.0
39.00	1823.0
39.90	230.0
43.90	713.0
45.00	904.0
46.00	183.0
46.90	1295.0
48.00	581.0
49.00	3770.0
50.00	18656.0
51.00	5586.0
52.00	277.0
52.90	101.0
55.00	295.0
56.00	1632.0
57.00	2789.0
58.00	156.0
60.00	897.0
61.00	4857.0
62.00	4948.0
63.00	3883.0
64.00	497.0
65.00	674.0
67.10	340.0
68.00	11091.0
69.00	10510.0
70.00	813.0
71.90	492.0
73.00	4944.0
74.00	18144.0
75.00	52760.0
76.00	4525.0
77.00	479.0
77.90	512.0
78.90	3926.0
80.00	1269.0
80.90	3868.0
81.90	799.0
83.00	112.0
86.00	160.0
87.00	3754.0
88.00	4094.0
90.90	492.0
92.00	3187.0
93.10	4859.0
94.00	12955.0
95.00	100432.0
96.10	6573.0
97.00	218.0
103.90	517.0
104.80	158.0
105.90	462.0
106.90	167.0
110.90	138.0
113.10	154.0
114.80	120.0
115.90	425.0
116.90	663.0
117.90	418.0
118.90	604.0
128.00	366.0
128.80	181.0
130.00	349.0
130.80	173.0
135.00	241.0
136.90	192.0
140.10	144.0
140.90	1147.0
141.80	176.0
142.90	1400.0
144.80	156.0
145.10	155.0
145.80	176.0
147.80	304.0
149.90	150.0
153.80	107.0
154.80	215.0
156.80	179.0
169.50	108.0
170.90	197.0
172.00	1059.0
174.00	77032.0
175.00	6117.0
176.00	74336.0
177.00	4486.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
36.00	740.0
37.00	4760.0
38.00	3663.0
39.00	1652.0
39.90	224.0
43.90	693.0
45.00	911.0
46.00	144.0
47.00	1186.0
47.90	603.0
49.00	3462.0
50.00	17512.0
51.00	5423.0
52.00	282.0
55.00	236.0
56.00	1541.0
57.00	2526.0
58.00	139.0
59.90	783.0
61.00	4813.0
62.00	4549.0
63.00	3688.0
63.90	431.0
65.00	630.0
67.10	326.0
68.00	10331.0
69.00	10127.0
70.00	785.0
71.80	521.0
73.00	4618.0
74.00	17112.0
75.00	49784.0
76.00	4189.0
76.90	497.0
77.90	476.0
78.90	3848.0
80.00	1144.0
80.90	3658.0
81.90	717.0
82.90	113.0
86.00	159.0
87.00	3750.0
88.00	3881.0
90.80	499.0
92.00	2904.0
93.10	4859.0
94.00	12355.0
95.00	94800.0
96.10	5862.0
97.00	211.0
103.90	457.0
104.80	124.0
105.90	422.0
106.90	137.0
112.00	110.0
113.00	140.0
114.90	151.0
115.90	356.0
116.90	646.0
117.90	467.0
118.90	584.0
127.90	376.0
128.80	192.0
130.00	363.0
130.80	169.0
135.00	199.0
136.80	228.0
140.10	148.0
140.90	1047.0
141.80	178.0
142.90	1328.0
144.30	129.0
144.70	133.0
145.90	145.0
147.90	255.0
149.90	151.0
154.90	217.0
156.80	187.0
170.90	218.0
172.00	980.0
173.00	1088.0
174.00	75152.0
175.00	5948.0
176.00	72544.0
177.00	4266.0
177.90	143.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63