

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV051320\
 Data File : VV016048.D
 Acq On : 13 May 2020 18:25
 Operator : SY/MD
 Sample : L2598-02
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H41X6

Quant Time: May 14 05:13:34 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu May 14 02:25:38 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	155236	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	155811	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	69807	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	51345	6.10	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	122.00%
7) Chloroethane-d5	1.58	69	47691	5.97	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	119.40%
11) 1,1-Dichloroethene-d2	2.13	63	74625	4.12	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.40%
20) 2-Butanone-d5	3.93	46	123890	51.57	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.14%
24) Chloroform-d	4.38	84	100373	5.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.00%
26) 1,2-Dichloroethane-d4	5.06	65	54627	5.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.60%
32) Benzene-d6	5.08	84	196745	5.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.20%
36) 1,2-Dichloropropane-d6	6.10	67	59492	5.26	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.20%
41) Toluene-d8	7.34	98	171316	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.80%
45) trans-1,3-Dichloropropene-	7.65	79	18691	4.21	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.20%
48) 2-Hexanone-d5	8.12	63	91390	46.84	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.68%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	40746	5.12	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.40%
65) 1,2-Dichlorobenzene-d4	11.65	152	62045	5.48	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.60%


Target Compounds					Ovalue
13) Acetone	2.22	43	5225	3.297 ug/L	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV051320\
Data File : VV016048.D
Acq On : 13 May 2020 18:25
Operator : SY/MD
Sample : L2598-02
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H41X6

Quant Time: May 14 05:13:34 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu May 14 02:25:38 2020
Response via : Initial Calibration

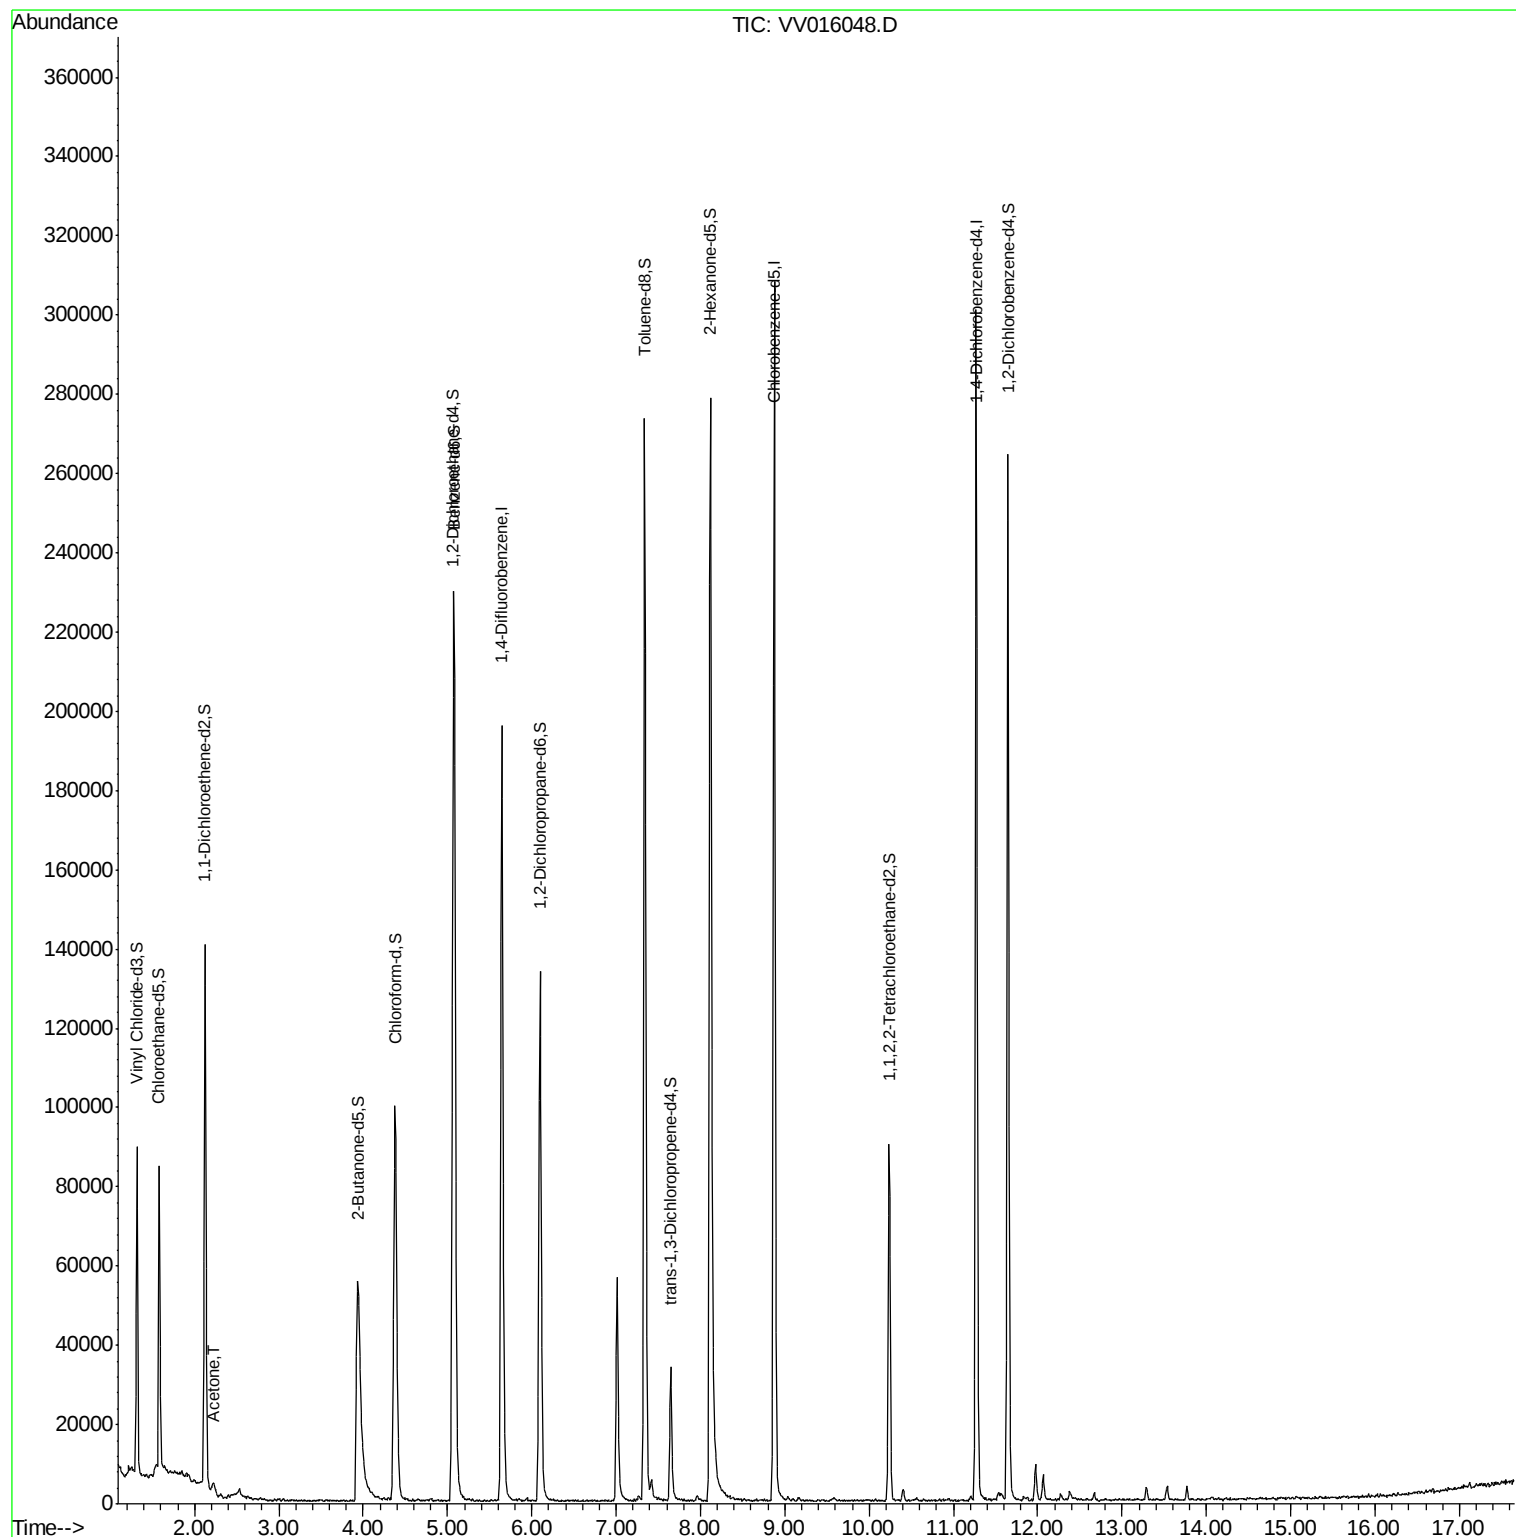

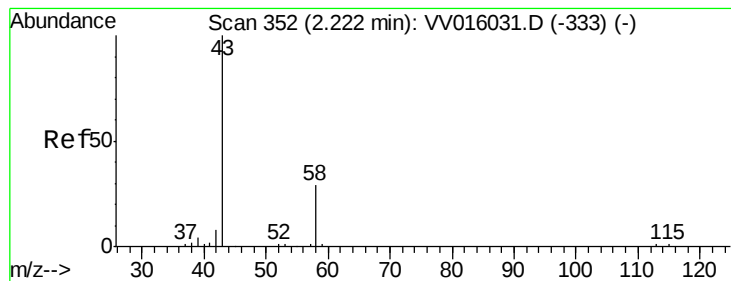

#13
 Acetone
 Concen: 3.297 ug/L
 RT: 2.22 min Scan# 351
 Delta R.T. -0.00 min
 Lab File: VV016048.D
 Acq: 13 May 2020 18:25

Instrument :
 MSVOA_V
 ClientSampleId :
 H41X6

Tot Ion: 43 Resp: 5225
 Ion Ratio Lower Upper
 43 100
 58 29.3 0.0 30.8

