


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV051320\
 Data File : VV016030.D
 Acq On : 13 May 2020 09:44
 Operator : SY/MD
 Sample : BFB56
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB56

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu May 14 02:25:38 2020

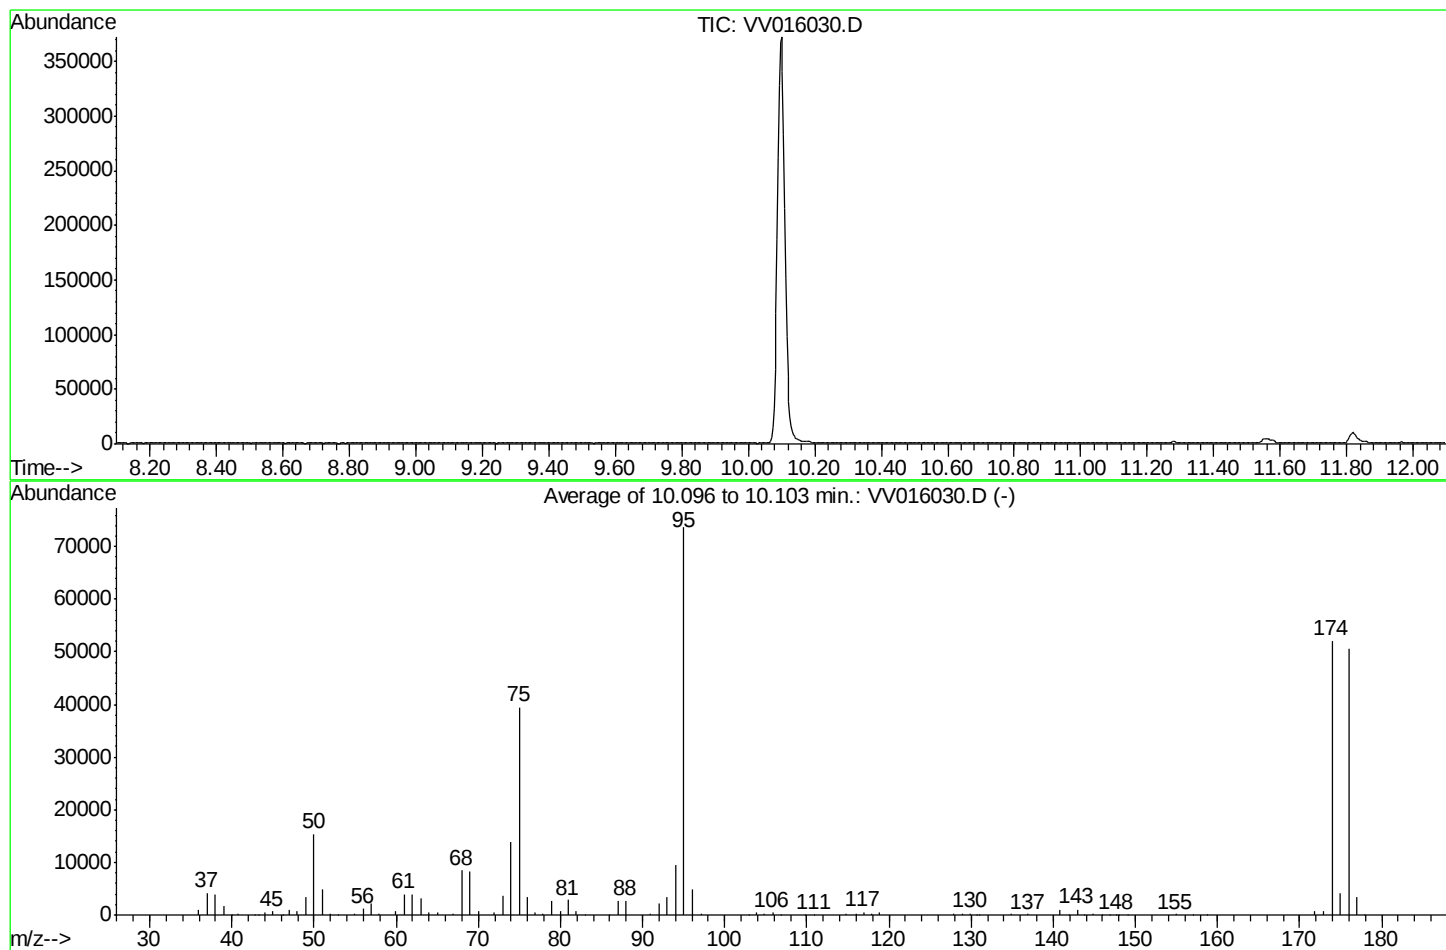

AutoFind: Scans 2801, 2802, 2803; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	15368	PASS
75	95	30	80	53.5	39410	PASS
95	95	100	100	100.0	73653	PASS
96	95	5	9	6.6	4877	PASS
173	174	0.00	2	1.5	790	PASS
174	95	50	120	70.8	52168	PASS
175	174	5	9	8.1	4224	PASS
176	174	95	101	97.1	50674	PASS
177	176	5	9	6.5	3307	PASS

m/z	Abundance
36.00	901.0
37.00	4691.0
38.00	3937.0
39.00	1911.0
40.00	431.0
40.80	131.0
42.80	108.0
44.00	870.0
45.00	738.0
46.20	170.0
47.00	955.0
48.00	588.0
49.00	3669.0
50.00	15872.0
51.00	4989.0
52.00	279.0
52.90	107.0
55.00	276.0
56.00	1309.0
57.00	2337.0
58.00	145.0
59.90	833.0
61.00	4132.0
62.00	4051.0
63.00	3433.0
64.00	426.0
65.00	535.0
66.90	338.0
68.00	8540.0
69.00	8468.0
70.00	762.0
71.90	440.0
73.00	3562.0
74.00	14216.0
75.00	40704.0
76.00	3631.0
76.90	497.0
77.90	342.0
78.90	2828.0
79.90	808.0
80.90	2909.0
81.90	721.0
87.00	2713.0
88.00	2986.0
90.80	399.0
92.00	2145.0
93.00	3488.0
94.00	9542.0
95.00	75720.0
96.00	5094.0
97.20	166.0
103.90	442.0
104.70	116.0
105.90	423.0
106.80	112.0
114.70	103.0
116.00	345.0
116.90	576.0
117.80	295.0
118.90	472.0
127.80	290.0
128.90	151.0
129.90	343.0
131.00	139.0
134.90	141.0
136.90	156.0
140.80	906.0
142.90	1008.0
143.80	105.0
144.90	222.0
145.90	107.0
147.70	188.0
154.90	153.0
156.90	111.0
158.70	114.0
171.90	713.0
173.00	804.0
173.90	52280.0
174.90	4289.0
175.90	50064.0
177.00	3343.0
177.90	130.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56

m/z	Abundance
36.00	903.0
37.00	4300.0
38.00	4044.0
39.00	1853.0
40.00	438.0
40.80	157.0
42.80	121.0
44.00	835.0
44.90	705.0
46.20	143.0
47.00	949.0
48.00	632.0
49.00	3526.0
50.00	15787.0
51.00	4994.0
52.00	281.0
52.90	124.0
54.90	260.0
56.00	1206.0
57.00	2320.0
58.00	140.0
59.90	844.0
61.00	4130.0
62.00	4011.0
63.00	3232.0
64.00	414.0
65.00	486.0
66.90	326.0
68.00	8771.0
69.00	8411.0
70.00	690.0
71.90	430.0
72.90	3707.0
74.00	14210.0
75.00	40968.0
76.00	3532.0
76.90	555.0
77.90	309.0
78.90	2739.0
79.90	775.0
80.90	2867.0
81.90	747.0
85.90	102.0
87.00	2776.0
87.90	2882.0
90.80	371.0
92.00	2133.0
93.00	3505.0
94.00	9750.0
95.00	76320.0
96.00	5054.0
97.20	164.0
102.90	103.0
103.90	451.0
104.80	144.0
105.80	475.0
106.80	108.0
109.70	108.0
110.90	100.0
114.70	152.0
116.00	381.0
116.90	627.0
117.90	314.0
118.90	461.0
127.90	288.0
129.00	151.0
129.90	331.0
130.90	139.0
134.90	138.0
136.90	173.0
140.80	952.0
142.00	122.0
142.90	1065.0
143.80	104.0
144.80	186.0
146.00	128.0
147.70	157.0
149.00	101.0
154.90	166.0
156.90	109.0
158.70	123.0
171.90	737.0
172.90	830.0
173.90	53688.0
174.90	4345.0
175.90	52408.0
177.00	3412.0
177.90	122.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56

m/z	Abundance
35.90	824.0
37.00	3592.0
38.00	3620.0
39.00	1663.0
40.00	463.0
40.80	154.0
42.80	124.0
43.30	112.0
44.00	821.0
44.90	629.0
47.00	890.0
47.90	639.0
49.00	3108.0
50.00	14445.0
51.00	4391.0
52.00	238.0
52.90	112.0
54.90	232.0
56.00	1042.0
57.00	2100.0
57.90	122.0
59.90	750.0
61.00	3749.0
62.00	3708.0
63.00	2858.0
64.00	389.0
65.00	423.0
66.90	298.0
68.00	7932.0
69.00	7659.0
70.00	614.0
71.90	375.0
72.90	3382.0
74.00	12840.0
75.00	36560.0
76.00	3119.0
76.90	537.0
77.90	278.0
78.90	2383.0
80.00	735.0
80.90	2655.0
81.90	719.0
82.90	119.0
85.90	121.0
87.00	2476.0
87.90	2521.0
90.90	328.0
92.00	2068.0
93.00	3203.0
94.00	9106.0
95.00	68920.0
96.00	4485.0
97.10	146.0
103.90	415.0
104.90	140.0
105.80	493.0
106.80	112.0
109.70	120.0
114.70	158.0
116.00	336.0
116.90	575.0
117.90	288.0
118.80	395.0
127.90	253.0
129.00	130.0
129.90	300.0
130.70	116.0
134.90	137.0
136.90	155.0
140.80	842.0
141.90	135.0
142.90	1013.0
144.70	156.0
146.00	141.0
146.90	109.0
147.90	125.0
154.90	176.0
157.00	115.0
158.70	103.0
171.80	689.0
172.90	736.0
173.90	50536.0
174.90	4040.0
176.00	49552.0
177.00	3168.0
177.80	116.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56

Scan 2788 (10.055 min): VV016030.D
BFB56

m/z	Abundance
39.80	319.0
44.00	377.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56