

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051324\
 Data File : VV035589.D
 Acq On : 13 May 2024 09:59
 Operator : SY/MD
 Sample : VV0513MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK295

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

Signal : TIC: VV035589.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	232571	251689	14.13%	1.889%
2	1.526	144	151	170	rVB	207094	255830	14.36%	1.920%
3	2.056	306	316	330	rBV	407066	588548	33.04%	4.416%
4	2.371	411	414	415	rBV2	539	311	0.02%	0.002%
5	2.445	429	437	449	rVB2	3627	6612	0.37%	0.050%
6	2.494	449	452	454	rBV2	439	239	0.01%	0.002%
7	2.699	508	516	531	rVB6	2193	4623	0.26%	0.035%
8	2.838	555	559	562	rBV2	224	219	0.01%	0.002%
9	2.892	573	576	578	rBV2	222	125	0.01%	0.001%
10	2.973	597	601	603	rBV	401	304	0.02%	0.002%
11	3.014	612	614	616	rBV2	238	122	0.01%	0.001%
12	3.037	619	621	623	rBV	105	64	0.00%	0.000%
13	3.111	634	644	648	rBV4	582	957	0.05%	0.007%
14	3.220	675	678	680	rBV2	178	139	0.01%	0.001%
15	3.272	691	694	698	rVB2	358	234	0.01%	0.002%
16	3.297	698	702	704	rBV2	110	76	0.00%	0.001%
17	3.320	708	709	714	rVB2	137	81	0.00%	0.001%
18	3.362	719	722	725	rVV2	327	194	0.01%	0.001%
19	3.381	725	728	734	rVV2	342	323	0.02%	0.002%
20	3.448	747	749	750	rBV	240	108	0.01%	0.001%
21	3.510	763	768	769	rBV	209	130	0.01%	0.001%
22	3.545	775	779	784	rVB2	322	289	0.02%	0.002%
23	3.571	785	787	790	rVB	225	133	0.01%	0.001%
24	3.587	790	792	795	rBV	184	97	0.01%	0.001%
25	3.629	802	805	809	rBV2	169	147	0.01%	0.001%
26	3.664	813	816	819	rVB	329	162	0.01%	0.001%
27	3.686	819	823	825	rVB	189	112	0.01%	0.001%
28	3.702	825	828	830	rBV	145	80	0.00%	0.001%
29	3.719	830	833	834	rBV	128	55	0.00%	0.000%
30	3.744	838	841	842	rBV	117	70	0.00%	0.001%
31	3.783	845	853	896	rBV	126397	371610	20.86%	2.789%
32	4.243	980	996	1027	rBV	285240	741955	41.65%	5.568%
33	4.715	1141	1143	1144	rBV	244	97	0.01%	0.001%
34	4.770	1158	1160	1163	rVB	176	98	0.01%	0.001%
35	4.854	1182	1186	1189	rBV2	260	259	0.01%	0.002%
36	4.953	1201	1217	1252	rBV2	670278	1781532	100.00%	13.368%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051324\
 Data File : VV035589.D
 Acq On : 13 May 2024 09:59
 Operator : SY/MD
 Sample : VV0513MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK295

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

37	5.436	1363	1367	1369	rBV3	424	331	0.02%	0.002%
38	5.529	1385	1396	1430	rBV	515068	1083156	60.80%	8.128%
39	5.825	1478	1488	1516	rVB3	34126	79278	4.45%	0.595%
40	5.985	1523	1538	1572	rBV	395874	832051	46.70%	6.244%
41	6.358	1651	1654	1657	rBV3	391	289	0.02%	0.002%
42	6.394	1661	1665	1669	rVB2	334	238	0.01%	0.002%
43	6.413	1669	1671	1674	rBV2	198	144	0.01%	0.001%
44	6.513	1701	1702	1706	rVB	279	140	0.01%	0.001%
45	6.551	1712	1714	1716	rBV	105	57	0.00%	0.000%
46	6.590	1721	1726	1728	rBV	243	177	0.01%	0.001%
47	6.606	1728	1731	1733	rBV	214	164	0.01%	0.001%
48	6.718	1762	1766	1768	rBV3	238	170	0.01%	0.001%
49	6.828	1796	1800	1804	rVB2	186	139	0.01%	0.001%
50	6.911	1809	1826	1861	rBV	181119	366646	20.58%	2.751%
51	7.239	1917	1928	1958	rBV	747937	1328878	74.59%	9.972%
52	7.551	2016	2025	2054	rBV	130414	250436	14.06%	1.879%
53	7.786	2094	2098	2107	rVB5	1087	1724	0.10%	0.013%
54	7.863	2119	2122	2123	rBV3	560	356	0.02%	0.003%
55	7.918	2132	2139	2150	rVB8	1951	3086	0.17%	0.023%
56	8.021	2161	2171	2214	rBV	412342	786000	44.12%	5.898%
57	8.593	2346	2349	2353	rBV3	308	326	0.02%	0.002%
58	8.619	2353	2357	2360	rBV3	411	301	0.02%	0.002%
59	8.667	2370	2372	2374	rBV2	335	175	0.01%	0.001%
60	8.693	2378	2380	2382	rBV	352	220	0.01%	0.002%
61	8.731	2390	2392	2394	rBV2	286	199	0.01%	0.001%
62	8.783	2397	2408	2441	rBV	795557	1331989	74.77%	9.995%
63	9.095	2496	2505	2507	rBV4	1642	2108	0.12%	0.016%
64	9.246	2550	2552	2557	rBV3	411	339	0.02%	0.003%
65	9.326	2576	2577	2578	rBV3	222	55	0.00%	0.000%
66	9.451	2610	2616	2618	rBV3	329	291	0.02%	0.002%
67	9.493	2621	2629	2635	rBV3	1411	2284	0.13%	0.017%
68	9.522	2636	2638	2640	rBV3	380	213	0.01%	0.002%
69	9.583	2655	2657	2659	rBV	162	55	0.00%	0.000%
70	9.615	2664	2667	2670	rBV	248	192	0.01%	0.001%
71	9.660	2679	2681	2682	rBV	359	151	0.01%	0.001%
72	9.709	2693	2696	2699	rBV2	276	213	0.01%	0.002%
73	9.767	2712	2714	2717	rVB2	251	111	0.01%	0.001%
74	9.783	2717	2719	2724	rBV2	199	129	0.01%	0.001%
75	9.850	2738	2740	2741	rBV	321	132	0.01%	0.001%
76	9.959	2769	2774	2777	rVB3	498	393	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051324\
 Data File : VV035589.D
 Acq On : 13 May 2024 09:59
 Operator : SY/MD
 Sample : VV0513MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK295

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

77	10.040	2793	2799	2801	rBV4	1018	1167	0.07%	0.009%
78	10.088	2810	2814	2817	rBV2	317	261	0.01%	0.002%
79	10.149	2821	2833	2862	rBV	552123	870419	48.86%	6.531%
80	10.439	2919	2923	2925	rBV2	288	245	0.01%	0.002%
81	10.480	2930	2936	2942	rVV4	1199	1598	0.09%	0.012%
82	10.631	2981	2983	2987	rBV	530	408	0.02%	0.003%
83	10.722	3009	3011	3015	rBV	290	151	0.01%	0.001%
84	10.837	3044	3047	3048	rBV2	242	122	0.01%	0.001%
85	10.860	3048	3054	3055	rBV4	1299	1270	0.07%	0.010%
86	10.927	3073	3075	3077	rBV	387	161	0.01%	0.001%
87	11.030	3105	3107	3112	rBV2	322	268	0.02%	0.002%
88	11.130	3130	3138	3144	rBV6	2522	4309	0.24%	0.032%
89	11.181	3144	3154	3185	rVV	709955	1117477	62.73%	8.385%
90	11.557	3256	3271	3312	rBV	757412	1208758	67.85%	9.070%
91	12.033	3416	3419	3420	rBV	315	206	0.01%	0.002%
92	12.303	3500	3503	3506	rBV	351	273	0.02%	0.002%
93	12.596	3585	3594	3607	rVB6	2810	5230	0.29%	0.039%
94	12.641	3607	3608	3610	rBV	344	193	0.01%	0.001%
95	12.869	3676	3679	3680	rBV2	439	216	0.01%	0.002%
96	13.056	3734	3737	3740	rVB2	437	249	0.01%	0.002%
97	13.072	3740	3742	3745	rBV	324	223	0.01%	0.002%
98	13.207	3777	3784	3791	rBV2	4161	5898	0.33%	0.044%
99	13.445	3851	3858	3874	rBV	9536	16719	0.94%	0.125%
100	13.683	3925	3932	3946	rBV5	5949	9700	0.54%	0.073%

Sum of corrected areas: 13326481




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051324\
Data File : VV035589.D
Acq On : 13 May 2024 09:59
Operator : SY/MD
Sample : VV0513MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK295

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

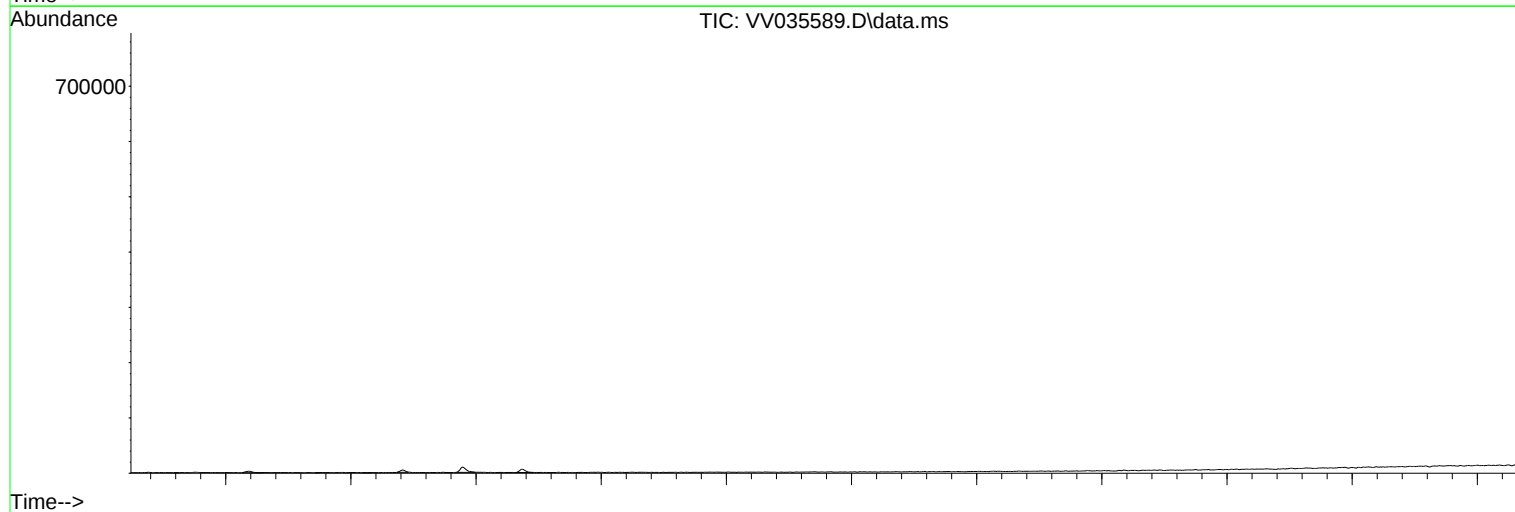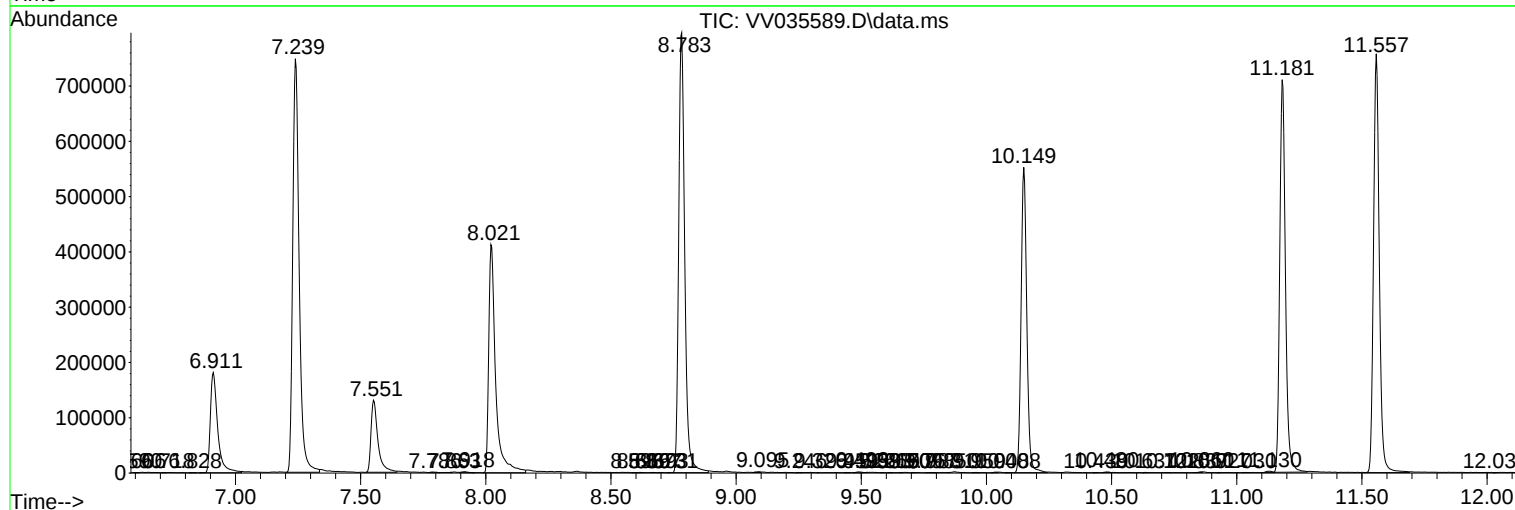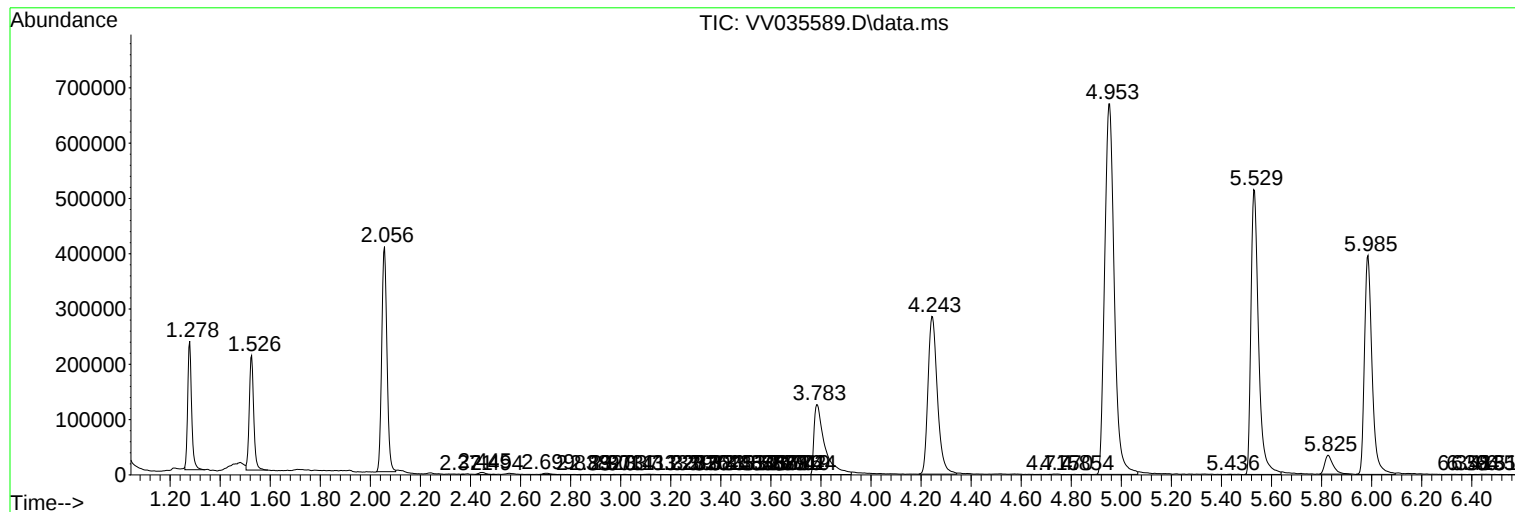

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051324\
Data File : VV035589.D
Acq On : 13 May 2024 09:59
Operator : SY/MD
Sample : VV0513MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK295

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051324\
Data File : VV035589.D
Acq On : 13 May 2024 09:59
Operator : SY/MD
Sample : VV0513MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK295

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------