

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051324\
 Data File : VV035590.D
 Acq On : 13 May 2024 10:23
 Operator : SY/MD
 Sample : VV0513WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK296

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

Signal : TIC: VV035590.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rVB	222084	239967	13.71%	1.836%
2	1.526	144	151	167	rVB	203409	245076	14.00%	1.875%
3	2.056	305	316	331	rBV	398498	578970	33.08%	4.430%
4	2.243	369	374	381	rVB5	1556	2147	0.12%	0.016%
5	2.394	414	421	426	rBV4	672	938	0.05%	0.007%
6	2.446	430	437	448	rVB3	3192	5475	0.31%	0.042%
7	2.555	464	471	477	rBV3	1786	2788	0.16%	0.021%
8	2.616	488	490	499	rVB2	300	386	0.02%	0.003%
9	2.703	509	517	527	rVV8	1938	3735	0.21%	0.029%
10	3.050	621	625	631	rVB3	333	362	0.02%	0.003%
11	3.085	631	636	639	rBV3	275	252	0.01%	0.002%
12	3.108	639	643	644	rBV	379	246	0.01%	0.002%
13	3.182	661	666	671	rBV2	422	382	0.02%	0.003%
14	3.333	711	713	719	rVB2	230	215	0.01%	0.002%
15	3.503	760	766	771	rBV2	338	361	0.02%	0.003%
16	3.783	845	853	897	rBV	126928	376056	21.48%	2.877%
17	4.243	980	996	1034	rBV2	280563	730086	41.71%	5.586%
18	4.577	1093	1100	1103	rBV5	1068	1264	0.07%	0.010%
19	4.661	1122	1126	1129	rVB3	656	576	0.03%	0.004%
20	4.680	1129	1132	1135	rBV2	369	377	0.02%	0.003%
21	4.728	1142	1147	1152	rBV2	565	684	0.04%	0.005%
22	4.953	1200	1217	1251	rBV2	658961	1750336	100.00%	13.393%
23	5.423	1360	1363	1368	rBV3	423	418	0.02%	0.003%
24	5.445	1368	1370	1374	rVB3	487	328	0.02%	0.003%
25	5.471	1374	1378	1380	rBV2	427	283	0.02%	0.002%
26	5.532	1385	1397	1429	rBV	497846	1053187	60.17%	8.059%
27	5.825	1477	1488	1513	rVV2	34828	80274	4.59%	0.614%
28	5.986	1525	1538	1573	rBV	388012	811995	46.39%	6.213%
29	6.182	1596	1599	1601	rBV4	834	396	0.02%	0.003%
30	6.275	1625	1628	1631	rVB3	599	355	0.02%	0.003%
31	6.339	1643	1648	1653	rVB3	224	323	0.02%	0.002%
32	6.439	1675	1679	1680	rBV	483	328	0.02%	0.003%
33	6.506	1696	1700	1703	rBV	474	265	0.02%	0.002%
34	6.532	1703	1708	1714	rVB2	357	340	0.02%	0.003%
35	6.641	1736	1742	1744	rVV4	535	538	0.03%	0.004%
36	6.748	1771	1775	1776	rBV3	364	239	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051324\
 Data File : VV035590.D
 Acq On : 13 May 2024 10:23
 Operator : SY/MD
 Sample : VV0513WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK296

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

37	6.770	1780	1782	1787	rVB2	367	270	0.02%	0.002%
38	6.912	1815	1826	1859	rBV	181588	360692	20.61%	2.760%
39	7.150	1895	1900	1901	rBV2	971	872	0.05%	0.007%
40	7.240	1916	1928	1953	rBV	732333	1302549	74.42%	9.967%
41	7.551	2014	2025	2053	rBV	129935	247336	14.13%	1.893%
42	7.760	2088	2090	2092	rBV2	358	220	0.01%	0.002%
43	7.780	2094	2096	2104	rVB5	1025	795	0.05%	0.006%
44	7.857	2116	2120	2121	rBV3	434	272	0.02%	0.002%
45	7.870	2122	2124	2127	rBV	395	272	0.02%	0.002%
46	7.908	2132	2136	2137	rBV	1418	1063	0.06%	0.008%
47	8.021	2162	2171	2217	rBV	410372	796187	45.49%	6.092%
48	8.358	2269	2276	2284	rBV9	1909	3347	0.19%	0.026%
49	8.439	2298	2301	2304	rVV2	353	211	0.01%	0.002%
50	8.458	2304	2307	2311	rBV4	291	255	0.01%	0.002%
51	8.574	2342	2343	2349	rBV2	246	271	0.02%	0.002%
52	8.783	2396	2408	2437	rBV	779186	1302877	74.44%	9.969%
53	9.040	2484	2488	2490	rBV5	368	230	0.01%	0.002%
54	9.066	2493	2496	2499	rVB4	393	230	0.01%	0.002%
55	9.092	2499	2504	2508	rBV4	1320	1522	0.09%	0.012%
56	9.149	2520	2522	2527	rVB4	420	304	0.02%	0.002%
57	9.307	2567	2571	2573	rBV2	265	235	0.01%	0.002%
58	9.445	2611	2614	2617	rVB2	371	214	0.01%	0.002%
59	9.474	2620	2623	2624	rBV	613	319	0.02%	0.002%
60	9.487	2624	2627	2632	rVB4	682	737	0.04%	0.006%
61	9.564	2647	2651	2654	rBV2	345	235	0.01%	0.002%
62	9.580	2654	2656	2662	rVB4	445	391	0.02%	0.003%
63	9.625	2665	2670	2677	rBV	271	326	0.02%	0.002%
64	9.677	2682	2686	2691	rVB2	486	447	0.03%	0.003%
65	9.876	2739	2748	2753	rBV4	1177	1800	0.10%	0.014%
66	9.973	2775	2778	2781	rBV2	300	262	0.01%	0.002%
67	10.047	2794	2801	2803	rBV	255	219	0.01%	0.002%
68	10.149	2821	2833	2859	rBV	548194	867439	49.56%	6.637%
69	10.323	2883	2887	2891	rBV3	900	710	0.04%	0.005%
70	10.391	2905	2908	2912	rVB2	275	229	0.01%	0.002%
71	10.419	2912	2917	2919	rBV2	340	273	0.02%	0.002%
72	10.436	2919	2922	2930	rVB3	592	649	0.04%	0.005%
73	10.471	2930	2933	2935	rBV2	726	578	0.03%	0.004%
74	10.860	3050	3054	3055	rBV2	480	374	0.02%	0.003%
75	11.130	3131	3138	3143	rBV4	1736	2529	0.14%	0.019%
76	11.182	3143	3154	3178	rBV	678563	1082857	61.87%	8.286%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051324\
 Data File : VV035590.D
 Acq On : 13 May 2024 10:23
 Operator : SY/MD
 Sample : VV0513WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK296

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

77	11.391	3217	3219	3224	rVB4	731	535	0.03%	0.004%
78	11.558	3258	3271	3295	rBV	728461	1171123	66.91%	8.961%
79	12.079	3431	3433	3439	rVB2	356	371	0.02%	0.003%
80	12.165	3456	3460	3462	rVB2	468	346	0.02%	0.003%
81	12.185	3462	3466	3468	rBV2	470	366	0.02%	0.003%
82	12.278	3492	3495	3498	rBV2	325	280	0.02%	0.002%
83	12.381	3524	3527	3531	rBV4	390	400	0.02%	0.003%
84	12.509	3561	3567	3572	rBV4	545	677	0.04%	0.005%
85	12.558	3579	3582	3586	rVB3	290	215	0.01%	0.002%
86	12.593	3586	3593	3603	rBV4	1525	2489	0.14%	0.019%
87	12.734	3633	3637	3642	rVB3	386	406	0.02%	0.003%
88	12.767	3642	3647	3649	rBV2	362	264	0.02%	0.002%
89	12.863	3673	3677	3680	rVB3	486	413	0.02%	0.003%
90	12.892	3682	3686	3689	rBV2	340	310	0.02%	0.002%
91	13.117	3753	3756	3761	rBV3	382	337	0.02%	0.003%
92	13.207	3777	3784	3798	rVB6	2793	4599	0.26%	0.035%
93	13.452	3850	3860	3871	rBV	4753	8300	0.47%	0.064%
94	13.551	3888	3891	3893	rVB2	525	292	0.02%	0.002%
95	13.683	3925	3932	3943	rVB5	2920	4442	0.25%	0.034%
96	13.728	3943	3946	3949	rBV2	607	388	0.02%	0.003%
97	13.863	3984	3988	3995	rBV4	739	1041	0.06%	0.008%
98	14.390	4149	4152	4155	rBV2	530	314	0.02%	0.002%
99	14.410	4155	4158	4159	rBV2	399	213	0.01%	0.002%
100	14.506	4184	4188	4191	rBV3	547	414	0.02%	0.003%

Sum of corrected areas: 13069081




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051324\
Data File : VV035590.D
Acq On : 13 May 2024 10:23
Operator : SY/MD
Sample : VV0513WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK296

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

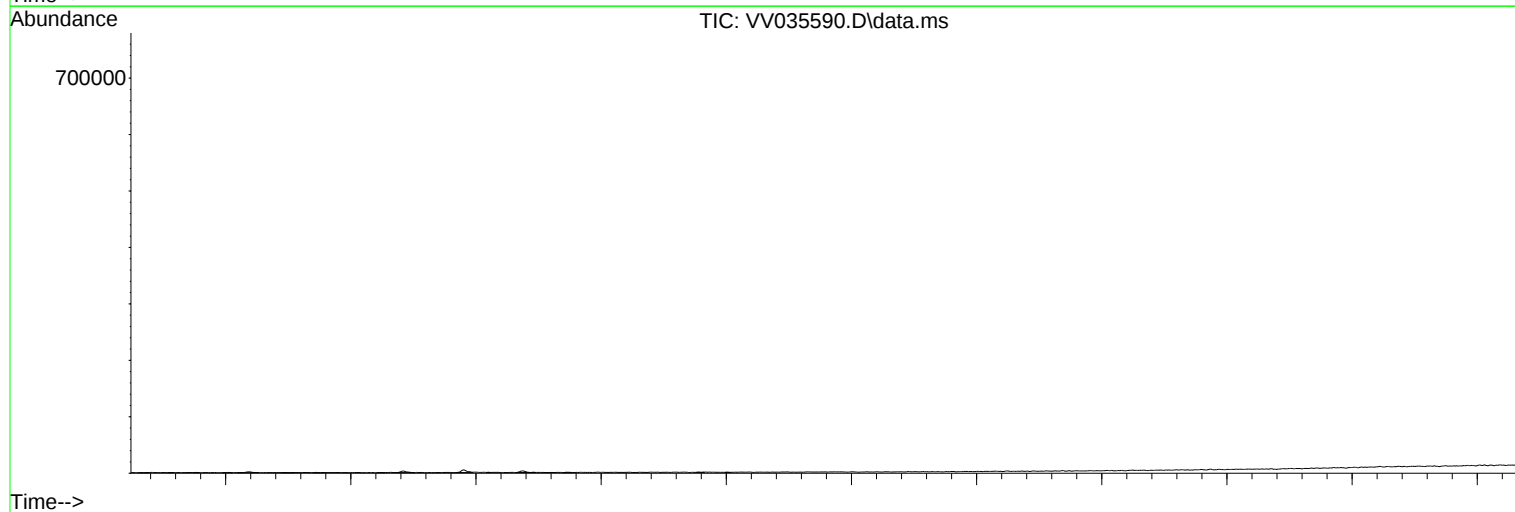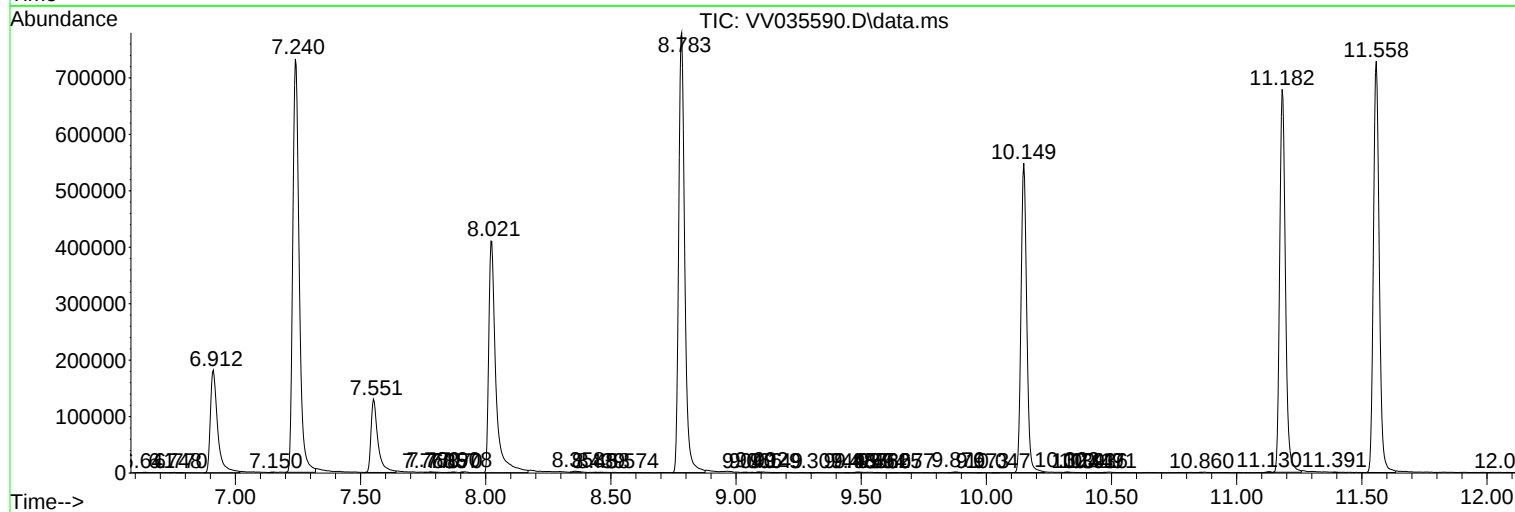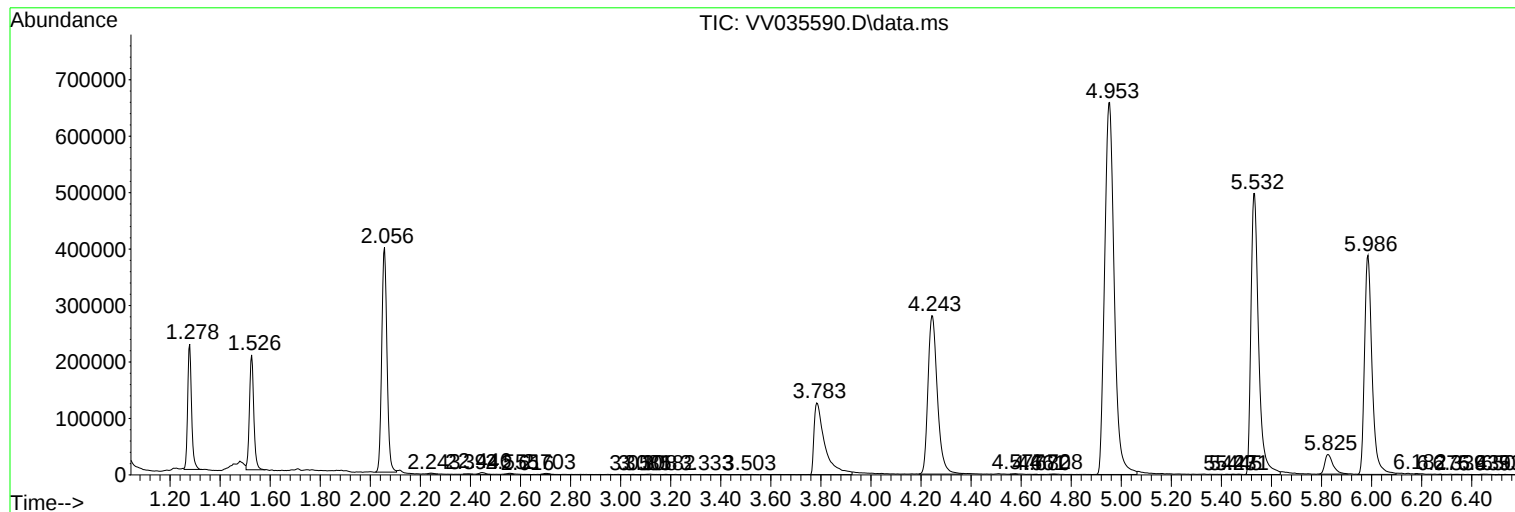

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051324\
Data File : VV035590.D
Acq On : 13 May 2024 10:23
Operator : SY/MD
Sample : VV0513WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK296

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051324\
Data File : VV035590.D
Acq On : 13 May 2024 10:23
Operator : SY/MD
Sample : VV0513WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK296

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------