
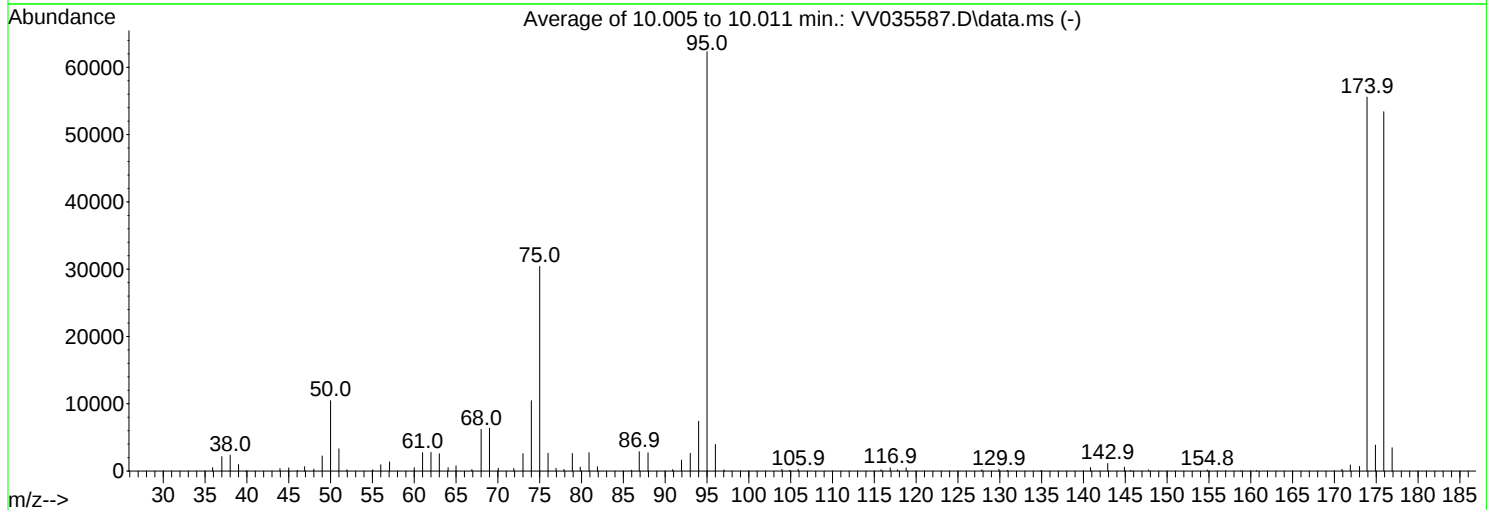


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051324\
Data File : VV035587.D
Acq On : 13 May 2024 08:19
Operator : SY/MD
Sample : BFB302
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB302

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Title : VOC Analysis
Last Update : Tue May 14 01:24:59 2024

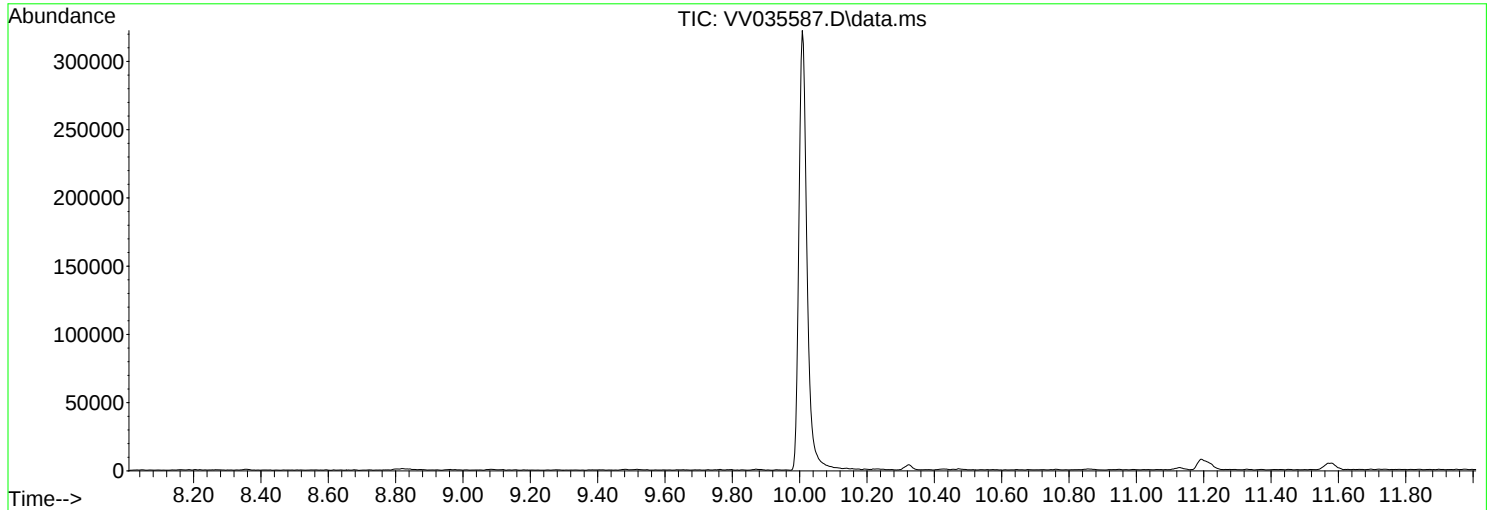

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	10467	PASS
75	95	30	80	48.8	30400	PASS
95	95	100	100	100.0	62317	PASS
96	95	5	9	6.3	3954	PASS
173	174	0.00	2	1.3	695	PASS
174	95	50	120	89.2	55579	PASS
175	174	5	9	7.0	3876	PASS
176	174	95	105	96.1	53400	PASS
177	176	5	10	6.5	3471	PASS

m/z	Abundance
40.00	184.0
44.00	381.0

Instrument :
MSVOA_V
ClientSampleId :
BFB302

m/z	Abundance
35.90	546.0
37.00	2136.0
38.00	2349.0
39.00	962.0
39.90	235.0
43.90	774.0
45.00	502.0
46.10	136.0
46.90	643.0
48.00	306.0
49.00	2239.0
50.00	10425.0
51.00	3172.0
52.00	219.0
55.00	241.0
56.00	799.0
57.00	1339.0
60.00	499.0
61.00	2658.0
62.00	2684.0
63.00	2590.0
64.00	531.0
65.00	878.0
66.90	257.0
68.00	6103.0
69.00	6118.0
70.10	409.0
71.90	394.0
73.00	2520.0
74.00	10221.0
75.00	30424.0
76.00	2724.0
77.00	363.0
77.90	231.0
78.90	2425.0
79.90	576.0
80.90	2750.0
81.90	583.0
86.00	143.0
86.90	2855.0
87.90	2474.0
90.90	242.0
91.90	1570.0
93.00	2559.0
94.00	7100.0
95.00	60208.0
96.00	3978.0
97.10	228.0
104.00	239.0
104.90	113.0
105.90	212.0
115.80	215.0
116.90	441.0
117.70	195.0
118.80	463.0
127.80	229.0
129.90	269.0
130.90	114.0
134.90	116.0
140.80	564.0
142.90	1127.0
144.90	554.0
145.60	127.0
147.80	176.0
154.80	120.0
170.90	251.0
171.90	854.0
173.00	595.0
173.90	52272.0
174.90	3982.0
175.90	49912.0
176.90	3281.0

Instrument :
MSVOA_V
ClientSampleId :
BFB302

m/z	Abundance
35.90	529.0
37.00	2257.0
38.00	2449.0
39.00	1004.0
39.80	250.0
43.90	779.0
45.00	491.0
46.00	129.0
46.90	693.0
48.00	317.0
49.00	2303.0
50.00	10867.0
51.00	3440.0
52.00	209.0
55.00	178.0
56.00	1001.0
57.10	1416.0
60.00	507.0
61.00	2791.0
62.00	2863.0
63.00	2642.0
64.10	520.0
65.00	797.0
66.90	260.0
68.00	6449.0
69.00	6595.0
70.10	420.0
71.90	381.0
73.00	2637.0
74.00	10795.0
75.00	31360.0
76.00	2762.0
76.90	418.0
77.90	254.0
78.90	2720.0
79.90	604.0
80.90	2863.0
81.90	686.0
86.00	125.0
86.90	2981.0
88.00	2775.0
90.90	223.0
92.00	1680.0
93.00	2792.0
94.00	7720.0
95.00	64272.0
96.00	4116.0
97.10	174.0
103.90	258.0
104.90	126.0
105.90	271.0
115.80	214.0
116.90	494.0
117.70	200.0
118.80	488.0
127.80	215.0
129.90	285.0
130.90	116.0
134.90	107.0
140.80	572.0
142.90	1179.0
144.90	611.0
145.60	126.0
147.80	196.0
154.80	188.0
157.00	101.0
160.70	111.0
170.90	297.0
171.90	928.0
173.00	738.0
173.90	57544.0
174.90	3966.0
175.90	55216.0
176.90	3545.0

Instrument :
MSVOA_V
ClientSampleId :
BFB302

m/z	Abundance
35.90	457.0
37.00	2066.0
38.00	2308.0
39.00	965.0
39.80	229.0
44.00	714.0
45.00	444.0
46.00	118.0
46.90	626.0
48.00	273.0
49.00	2192.0
50.00	10109.0
51.00	3324.0
51.90	170.0
55.10	157.0
56.00	1021.0
57.10	1353.0
60.00	529.0
61.00	2773.0
62.00	2776.0
63.00	2493.0
64.10	487.0
65.00	688.0
66.90	195.0
68.00	6054.0
69.00	6418.0
70.00	441.0
71.90	355.0
73.00	2638.0
74.00	10371.0
75.00	29416.0
76.00	2472.0
76.90	463.0
77.90	261.0
78.90	2685.0
79.80	608.0
80.90	2619.0
81.90	687.0
85.90	111.0
86.90	2808.0
88.00	2937.0
90.90	209.0
92.00	1658.0
93.00	2588.0
94.00	7401.0
95.00	62472.0
96.00	3768.0
97.00	140.0
103.90	251.0
104.90	131.0
105.90	302.0
115.80	187.0
116.90	524.0
117.80	200.0
118.80	452.0
127.90	197.0
129.90	286.0
130.90	124.0
140.90	471.0
142.90	1087.0
144.90	609.0
145.80	121.0
147.80	182.0
154.80	216.0
158.80	119.0
160.70	114.0
170.90	283.0
171.90	955.0
173.00	752.0
173.90	56920.0
174.90	3679.0
175.90	55072.0
176.90	3587.0

Instrument :
MSVOA_V
ClientSampleId :
BFB302