


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV051420\
Data File : VV016074.D
Acq On : 14 May 2020 18:08
Operator : SY/MD
Sample : L2661-01
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4246

Manual Integrations
APPROVED

apatel
5/15/2020 11:08:30 AM

Quant Time: May 15 08:27:40 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri May 15 06:27:04 2020
Response via : Initial Calibration

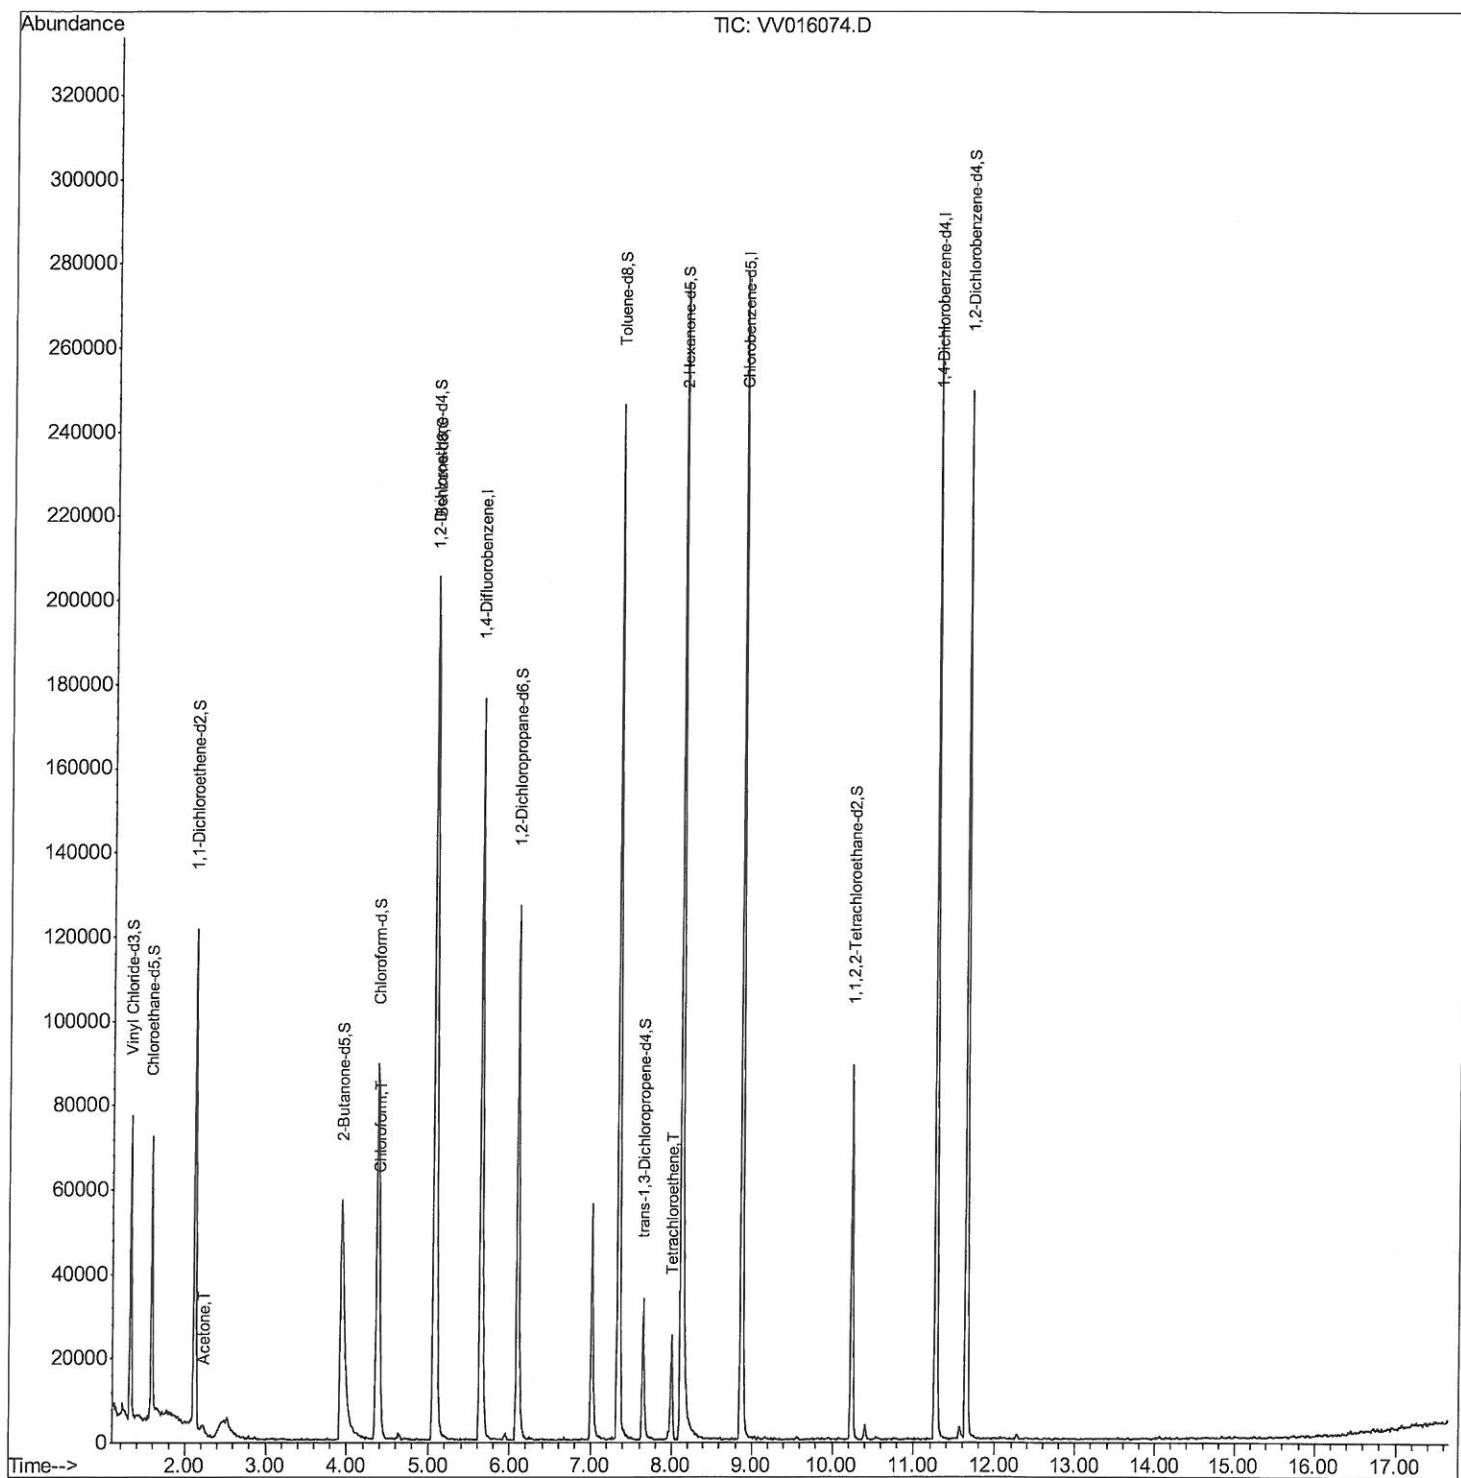

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV051420\
Data File : VV016074.D
Acq On : 14 May 2020 18:08
Operator : SY/MD
Sample : L2661-01
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 19 Sample Multiplier: 1

apatel
5/15/2020 11:08:30 AM

Abundance

Ion 43.05 (42.75 to 43.75): VV016074.D
Ion 58.05 (57.75 to 58.75): VV016074.D

Time-->

1

2d

3d

4d



5d

6d

7d

8d

9d

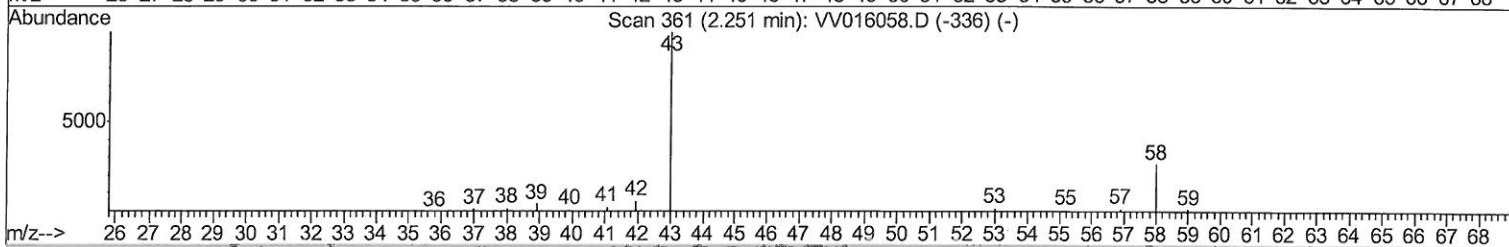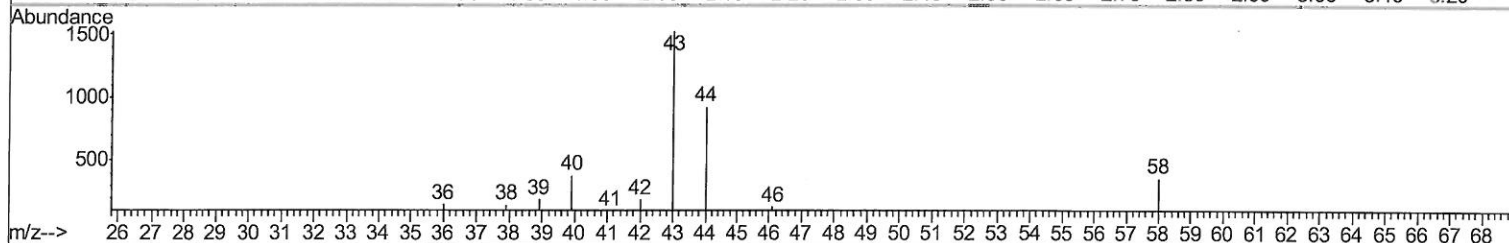

Ion	Exp%	Act%
43.05	100	100
58.05	15.40	28.87
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV051420\
Data File : VV016074.D
Acq On : 14 May 2020 18:08
Operator : SY/MD
Sample : L2661-01
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
H4246

Manual Integrations
APPROVED

apatel
5/15/2020 11:08:30 AM

Quant Time: May 15 06:31:36 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri May 15 06:27:04 2020
Response via : Initial Calibration

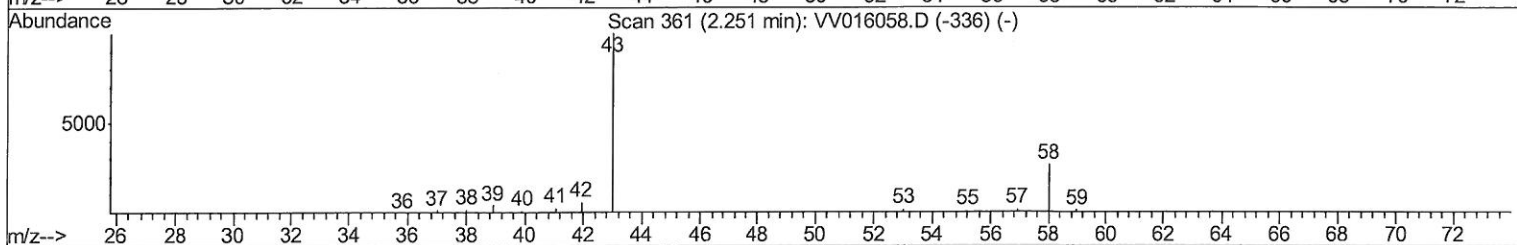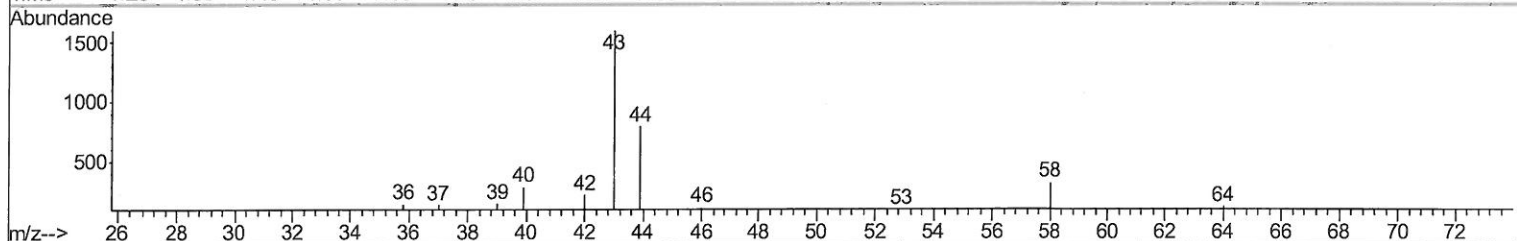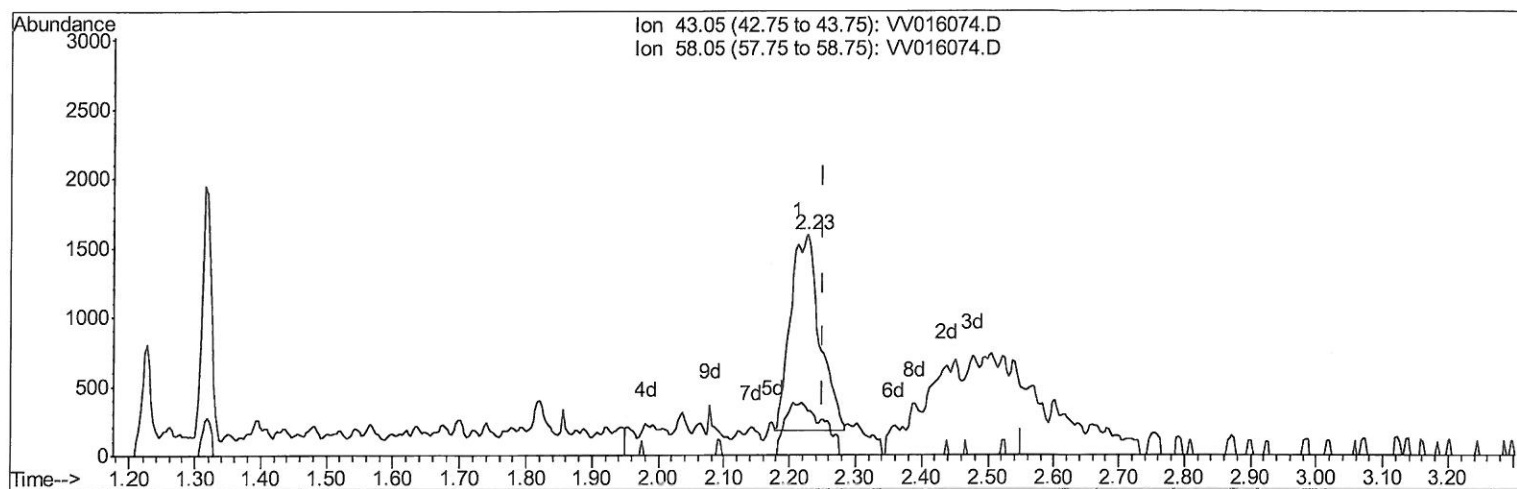

TIC: VV016074.D

(13) Acetone (T)

2.228min (-0.022) 3.05ug/L m

response 4341

Ion	Exp%	Act%
43.05	100	100
58.05	15.40	12.32
0.00	0.00	0.00
0.00	0.00	0.00

SY/MD
5/15/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV051420\
 Data File : VV016074.D
 Acq On : 14 May 2020 18:08
 Operator : SY/MD
 Sample : L2661-01
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4246

Manual Integrations
 APPROVED

apatel
 5/15/2020 11:08:30 AM

Quant Time: May 15 08:27:40 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri May 15 06:27:04 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	139308	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	140196	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	63173	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	42158	5.58	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	111.60%
7) Chloroethane-d5	1.58	69	42133	5.88	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	117.60%
11) 1,1-Dichloroethene-d2	2.13	63	64796	3.99	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.80%
20) 2-Butanone-d5	3.94	46	128418	59.57	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	119.14%
24) Chloroform-d	4.38	84	88574	5.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.20%
26) 1,2-Dichloroethane-d4	5.06	65	52634	5.56	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	111.20%
32) Benzene-d6	5.08	84	173077	5.19	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.80%
36) 1,2-Dichloropropane-d6	6.10	67	55744	5.48	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	109.60%
41) Toluene-d8	7.34	98	153021	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.00%
45) trans-1,3-Dichloropropene-	7.65	79	17832	4.46	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.20%
48) 2-Hexanone-d5	8.12	63	92980	52.96	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.92%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	40049	5.59	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	111.80%
65) 1,2-Dichlorobenzene-d4	11.65	152	57813	5.64	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	112.80%

Target Compounds

					Ovalue
13) Acetone	2.23	43	4341m	3.053	ug/L
25) Chloroform	4.41	83	7128	0.397	ug/L
49) Tetrachloroethene	8.00	164	5198	0.740	ug/L

2 MD
 5/15/20

(#) = qualifier out of range (m) = manual integration (+) = signals summed