


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV051420\
 Data File : VV016057.D
 Acq On : 14 May 2020 09:02
 Operator : SY/MD
 Sample : BFB57
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB57

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri May 15 06:27:04 2020

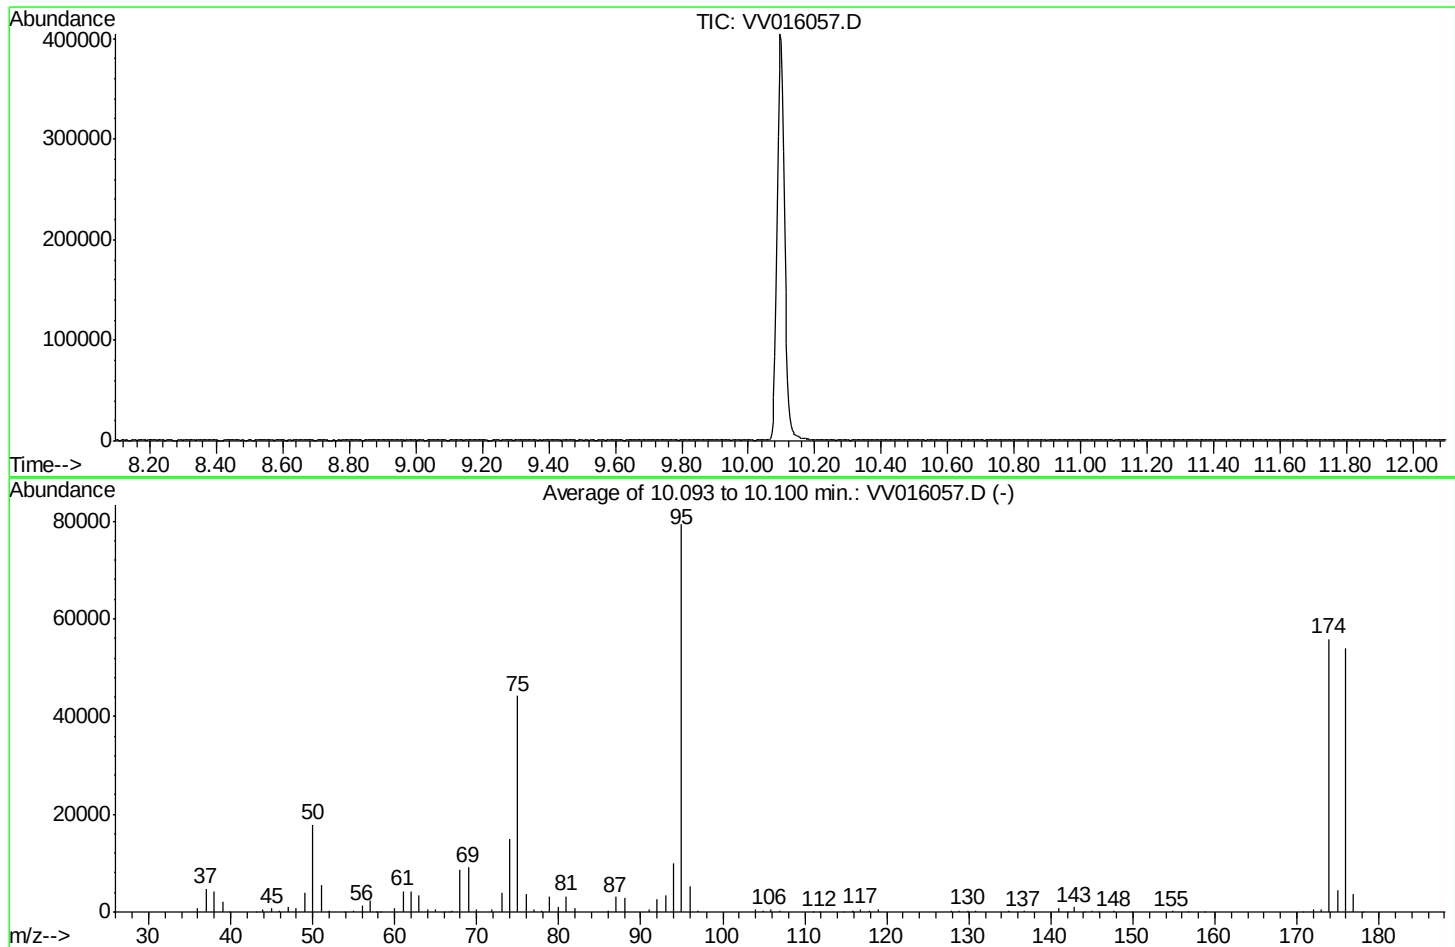

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.5	17864	PASS
75	95	30	80	55.7	44165	PASS
95	95	100	100	100.0	79344	PASS
96	95	5	9	6.6	5269	PASS
173	174	0.00	2	0.8	468	PASS
174	95	50	120	70.4	55861	PASS
175	174	5	9	8.1	4535	PASS
176	174	95	101	96.6	53984	PASS
177	176	5	9	6.6	3558	PASS

m/z	Abundance
36.00	867.0
37.00	4558.0
38.00	3996.0
39.00	2022.0
39.90	404.0
43.00	107.0
44.10	890.0
45.00	705.0
46.00	183.0
47.00	1090.0
48.00	733.0
49.00	3692.0
50.00	17328.0
51.00	5471.0
52.10	289.0
54.90	254.0
56.00	1211.0
57.00	2359.0
57.80	139.0
59.90	835.0
61.00	4155.0
62.00	3978.0
63.00	3358.0
64.00	537.0
65.00	491.0
66.90	249.0
68.00	8257.0
69.00	8792.0
70.00	689.0
71.90	616.0
73.00	3695.0
74.00	13948.0
75.00	41616.0
76.00	3460.0
77.00	536.0
78.00	286.0
78.90	3095.0
80.00	959.0
80.90	2941.0
81.90	802.0
86.00	196.0
86.90	3082.0
88.00	2814.0
91.00	428.0
92.00	2331.0
93.00	3264.0
94.00	9512.0
95.00	75664.0
96.00	4948.0
97.00	172.0
103.90	359.0
104.90	165.0
105.90	403.0
106.90	115.0
111.00	111.0
114.80	109.0
115.80	300.0
115.90	294.0
116.80	707.0
117.80	298.0
118.90	474.0
127.80	236.0
128.90	202.0
129.90	286.0
130.80	168.0
134.90	144.0
136.70	195.0
141.00	853.0
142.90	984.0
145.00	154.0
145.80	137.0
147.80	149.0
149.90	107.0
154.80	128.0
156.80	108.0
170.90	138.0
171.90	577.0
172.90	677.0
173.90	51080.0
175.00	4354.0
176.00	50192.0
176.90	3342.0

Instrument :
MSVOA_V
ClientSampleId :
BFB57

m/z	Abundance
36.00	869.0
37.00	4940.0
38.00	4188.0
39.00	2103.0
39.90	402.0
43.10	121.0
44.00	920.0
45.00	779.0
45.90	198.0
47.00	1173.0
48.00	761.0
49.00	3980.0
50.00	18576.0
51.00	5763.0
52.10	264.0
54.90	260.0
56.00	1316.0
57.00	2442.0
57.80	126.0
59.90	902.0
61.00	4469.0
62.00	4433.0
63.00	3631.0
64.00	539.0
65.00	517.0
66.00	118.0
67.00	226.0
68.00	8953.0
69.00	9405.0
70.00	651.0
71.90	629.0
73.00	4060.0
74.00	15399.0
75.00	45872.0
76.00	3661.0
76.90	587.0
78.00	266.0
78.90	3313.0
80.00	1014.0
80.90	3335.0
81.90	861.0
86.00	214.0
87.00	3133.0
88.00	3050.0
90.90	459.0
92.00	2651.0
93.00	3651.0
94.00	10376.0
95.00	82368.0
96.00	5459.0
97.00	176.0
103.90	443.0
104.90	179.0
105.90	430.0
106.90	158.0
111.80	102.0
114.70	105.0
115.80	296.0
116.80	674.0
117.90	360.0
118.90	524.0
127.80	288.0
128.80	211.0
129.90	327.0
130.80	173.0
134.90	167.0
136.80	227.0
140.90	958.0
142.90	1022.0
145.00	164.0
145.80	124.0
147.70	140.0
149.80	112.0
154.80	165.0
156.80	116.0
158.80	105.0
170.80	120.0
171.90	638.0
172.90	729.0
173.90	57744.0
175.00	4710.0
176.00	55776.0
176.90	3675.0

Instrument :
MSVOA_V
ClientSampleId :
BFB57

m/z	Abundance
35.90	815.0
37.00	4869.0
38.00	4052.0
39.00	2001.0
39.90	419.0
43.00	113.0
44.00	903.0
45.00	808.0
45.90	172.0
47.00	1167.0
47.90	696.0
49.00	3923.0
50.00	17688.0
51.00	5388.0
51.90	230.0
53.90	113.0
55.00	265.0
56.00	1254.0
57.00	2343.0
57.90	105.0
58.20	107.0
60.00	861.0
61.00	4258.0
62.00	4420.0
63.00	3411.0
64.00	528.0
65.00	552.0
66.00	122.0
66.70	192.0
67.10	199.0
68.00	8789.0
69.00	9130.0
70.00	618.0
71.90	552.0
73.00	3952.0
74.00	15415.0
75.00	45008.0
76.00	3603.0
76.90	556.0
77.90	245.0
78.90	3229.0
80.00	953.0
80.90	3451.0
81.90	786.0
86.00	177.0
87.00	2950.0
88.00	2905.0
90.90	421.0
92.00	2630.0
93.00	3655.0
94.00	10162.0
95.00	80000.0
96.00	5400.0
97.00	179.0
103.90	432.0
104.90	193.0
105.80	432.0
106.90	169.0
111.80	107.0
115.80	257.0
116.80	608.0
117.90	385.0
118.90	531.0
127.80	347.0
128.80	184.0
129.90	374.0
130.80	142.0
135.00	175.0
136.80	259.0
140.90	959.0
142.10	101.0
142.90	1007.0
144.10	104.0
144.80	183.0
145.90	126.0
147.70	133.0
149.80	123.0
154.80	184.0
156.80	140.0
158.80	110.0
170.80	100.0
172.00	661.0
173.90	58760.0
175.00	4542.0
176.00	55984.0
176.90	3659.0
178.10	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB57

Scan 2788 (10.055 min): VV016057.D
BFB57

m/z	Abundance
39.90	344.0
40.70	117.0
43.90	481.0

Instrument :
MSVOA_V
ClientSampleId :
BFB57