


Data Path : W:\HPCHEM1\MSVOA_V\DATA\VV051518\
Data File : VV005922.D
Acq On : 15 May 2018 18:15
Operator : SY/MD
Sample : J2905-18
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1




Quant Time: May 16 04:32:18 2018
Quant Method : W:\HPCHEM1\MSVOA_V\METHOD\SOMVTR050518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed May 16 03:06:39 2018
Response via : Initial Calibration

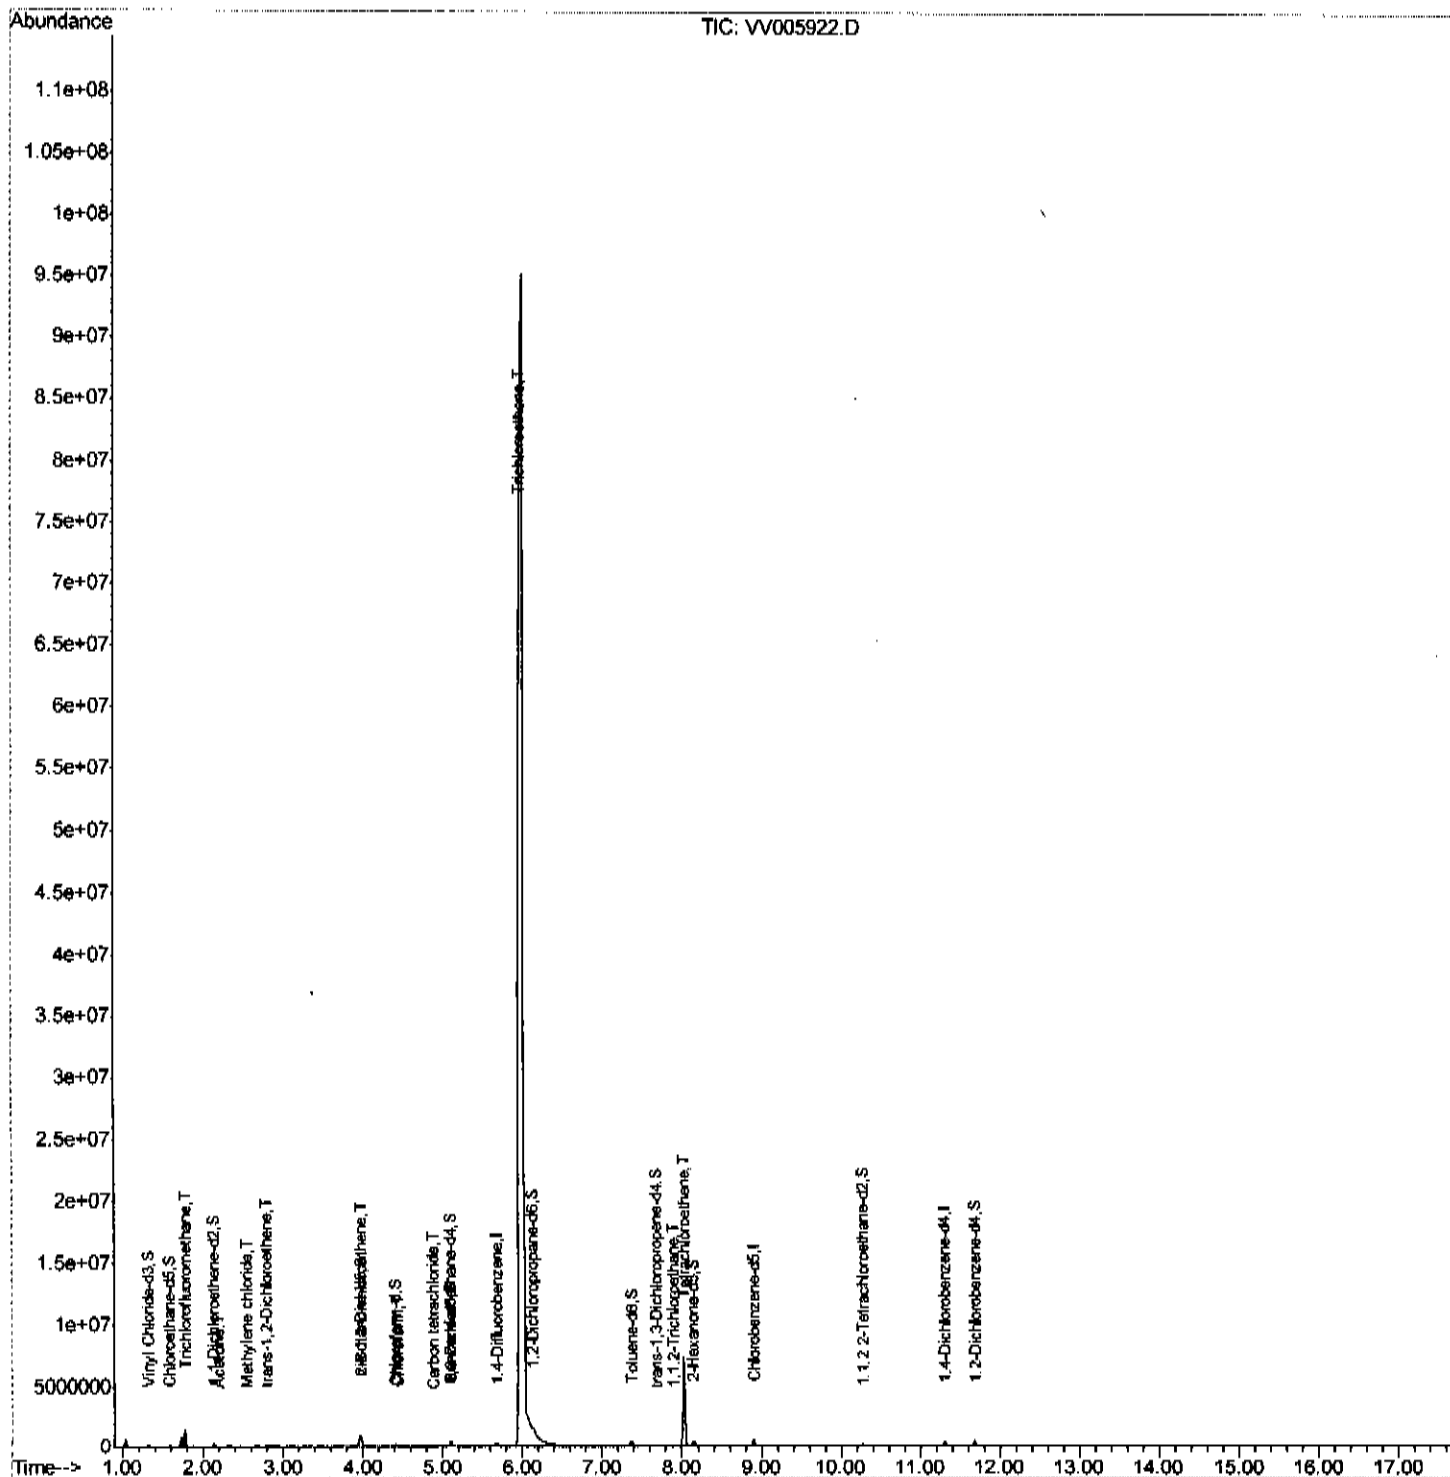

Quantitation Report (Qedit)

Data Path : W:\HPCHEM1\MSVOA_V\DATA\VV051518\
 Data File : VV005922.D
 Acq On : 15 May 2018 18:15
 Operator : SY/MD
 Sample : J2905-18
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 03:12:17 2018
 Quant Method : W:\HPCHEM1\MSVOA_V\METHOD\SOMVTR050518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed May 16 03:06:39 2018
 Response via : Initial Calibration

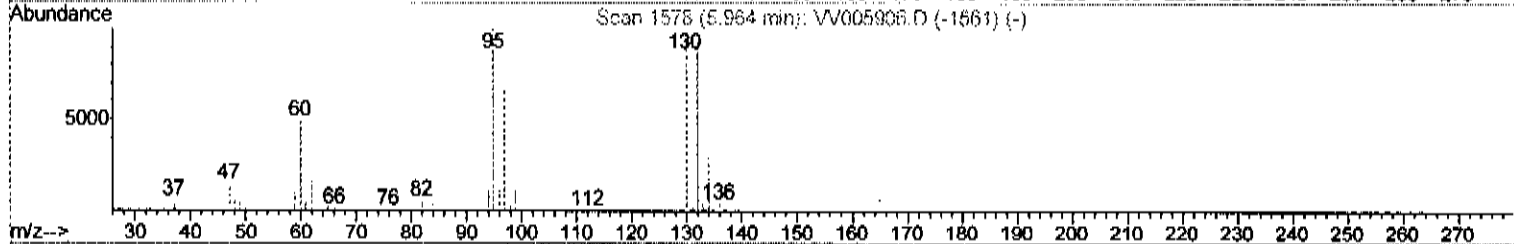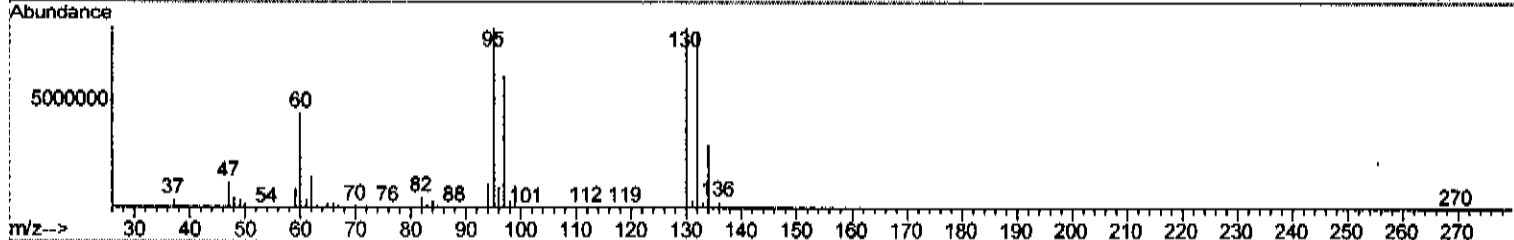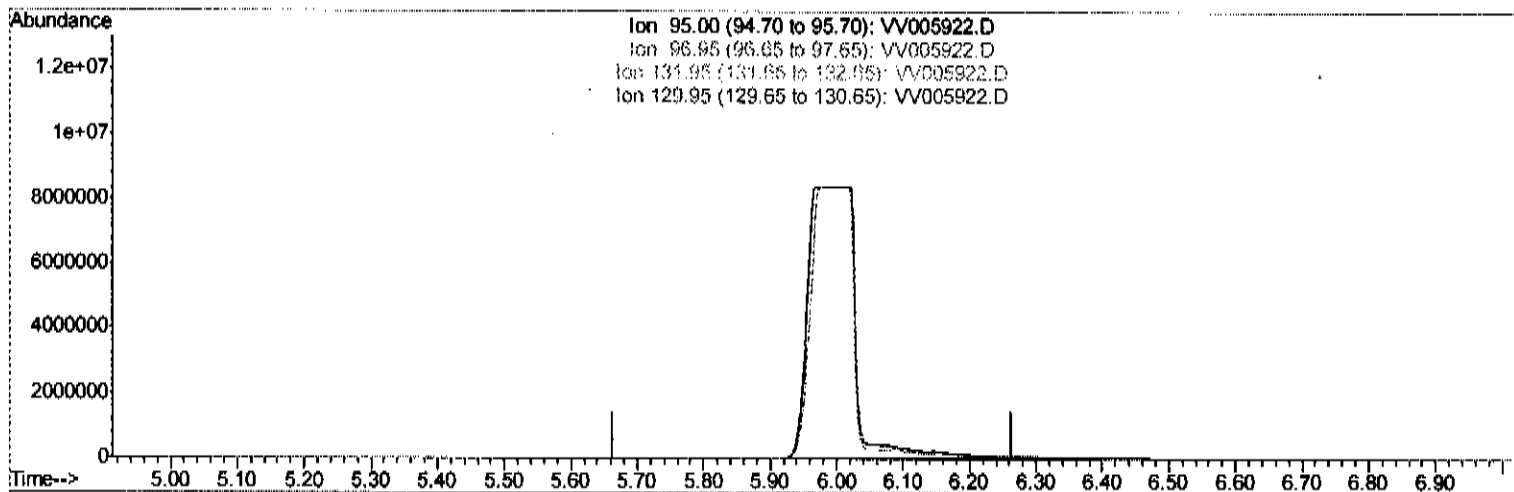

TIC: VV005922.D

(34) Trichloroethene (T)

5.964min (-5.964) 0.00ug/L




response 0

Ion	Exp%	Act%
95.00	100	0.00
96.95	65.20	0.00#
131.95	91.70	0.00#
129.95	98.60	0.00#

Quantitation Report (Qedit)

Data Path : W:\HPCHEM1\MSVOA_V\DATA\VV051518\
 Data File : VV005922.D
 Acq On : 15 May 2018 18:15
 Operator : SY/MD
 Sample : J2905-18
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 03:12:17 2018
 Quant Method : W:\HPCHEM1\MSVOA_V\METHOD\SOMVTR050518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed May 16 03:06:39 2018
 Response via : Initial Calibration

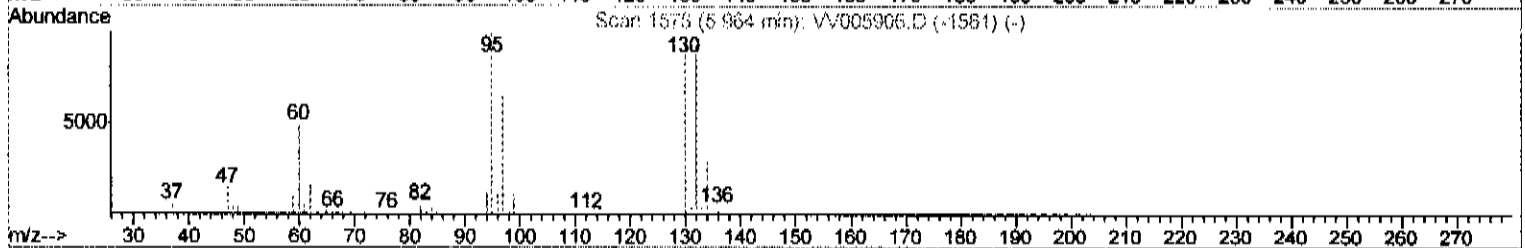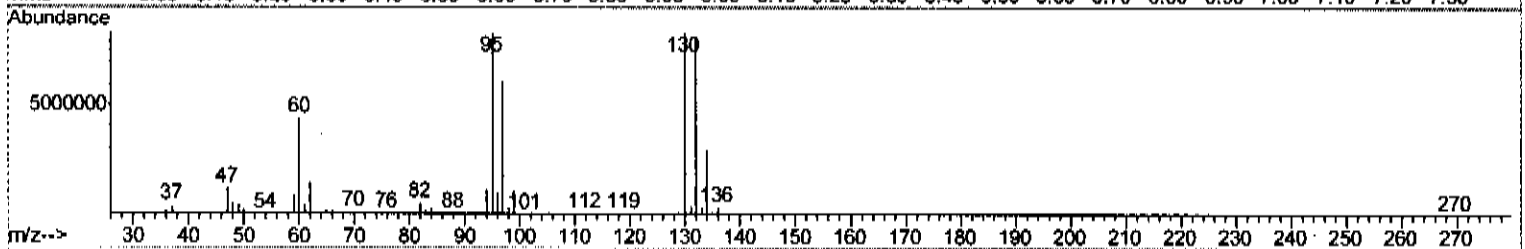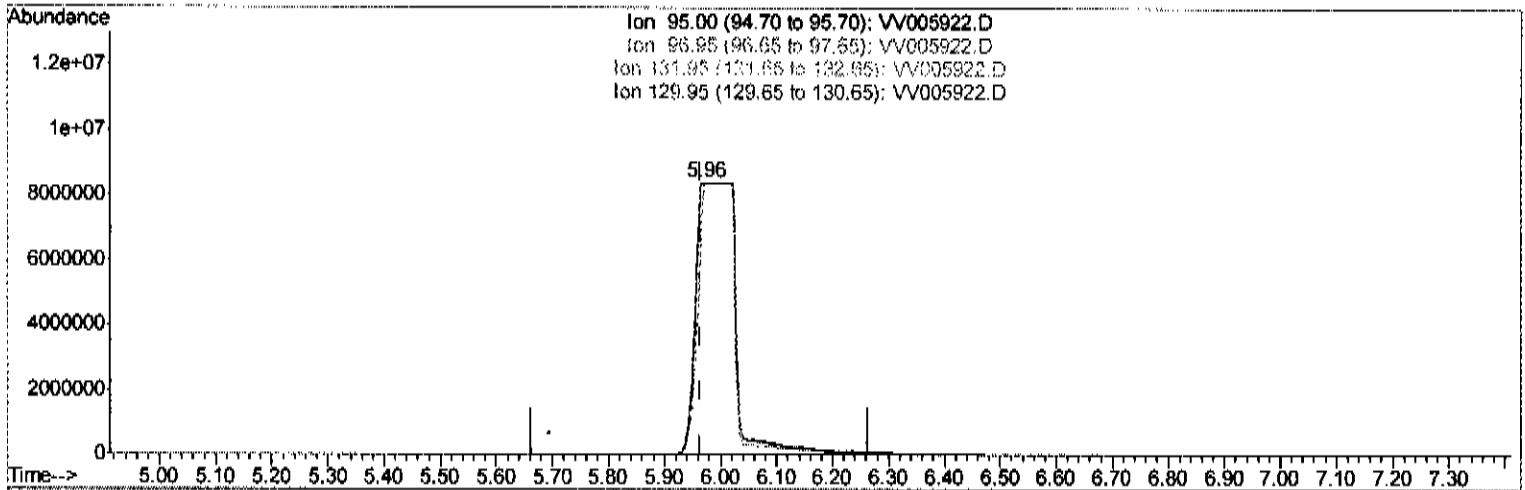

(34) Trichloroethene (T)

5.964min (-0.000) 1710.61ug/L m

response 42247390

Ion	Exp%	Act%
95.00	100	100
96.95	65.20	73.42
131.95	91.70	96.61
129.95	98.60	100.00

5/17/18 Sy

Data Path : W:\HPCHEM1\MSVOA_V\DATA\VV051518\
 Data File : VV005922.D
 Acq On : 15 May 2018 18:15
 Operator : SY/MD
 Sample : J2905-18
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 04:32:18 2018
 Quant Method : W:\HPCHEM1\MSVOA_V\METHOD\SOMVTR050518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed May 16 03:06:39 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	293121	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	298315	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	121741	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	88959	4.00	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.00%
7) Chloroethane-d5	1.58	69	81754	4.26	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.20%
11) 1,1-Dichloroethene-d2	2.13	63	136945	2.79	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	55.80%#
20) 2-Butanone-d5	3.96	46	247286	56.50	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.00%
24) Chloroform-d	4.41	84	207553	5.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.40%
26) 1,2-Dichloroethane-d4	5.09	65	112714	4.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.80%
32) Benzene-d6	5.11	84	371759	4.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.80%
36) 1,2-Dichloropropane-d6	6.13	67	125723	5.06	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.20%
41) Toluene-d8	7.37	98	339057	4.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.80%
43) trans-1,3-Dichloropropene-	7.67	79	43225	4.40	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.00%
46) 2-Hexanone-d5	8.14	63	176204	45.97	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.94%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	81044	4.34	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	120434	4.76	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.20%

Target Compounds

						Qvalue
9) Trichlorofluoromethane	1.77	101	911912	21.72	ug/L	100
13) Acetone	2.20	43	25355	6.84	ug/L	92
16) Methylene chloride	2.54	84	7221	0.31	ug/L	98
18) trans-1,2-Dichloroethene	2.79	96	47557	2.06	ug/L	95
22) cis-1,2-Dichloroethene	3.97	96	512446	22.65	ug/L	100
25) Chloroform	4.44	83	29287	0.62	ug/L	94
31) Carbon tetrachloride	4.88	117	13125	0.38	ug/L	95
34) Trichloroethene	5.96	95	42247390m	1710.61	ug/L	95
45) 1,1,2-Trichloroethane	7.89	97	11067	0.69	ug/L	95
47) Tetrachloroethene	8.03	164	1560874	90.10	ug/L	98

05/17/18 by

(#) = qualifier out of range (m) = manual integration (+) = signals summed