

Data Path : W:\HPCHEM1\MSVOA V\DATA\VV051518\
 Data File : VV005908.D
 Acq On : 15 May 2018 11:34
 Operator : SY/MD
 Sample : J2658-11
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 03:46:05 2018
 Quant Method : W:\HPCHEM1\MSVOA V\METHOD\SOMVTR050518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed May 16 03:06:39 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	397634	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	391800	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	156656	5.00	ug/L	0.00

System Monitoring Compounds


4) Vinyl Chloride-d3	1.32	65	122365	4.05	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.00%
7) Chloroethane-d5	1.59	69	97419	3.74	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	74.80%
11) 1,1-Dichloroethene-d2	2.13	63	176176	2.65	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	53.00%#
20) 2-Butanone-d5	3.96	46	198516	33.44	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	66.88%
24) Chloroform-d	4.41	84	182902	3.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	66.40%#
26) 1,2-Dichloroethane-d4	5.09	65	118399	3.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	72.60%
32) Benzene-d6	5.11	84	430291	4.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.80%
36) 1,2-Dichloropropane-d6	6.12	67	133998	4.10	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	82.00%
41) Toluene-d8	7.37	98	379831	3.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.00%
43) trans-1,3-Dichloropropene-	7.67	79	45094	3.50	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	70.00%
46) 2-Hexanone-d5	8.14	63	144707	28.74	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	57.48%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	79134	3.23	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	64.60%#
64) 1,2-Dichlorobenzene-d4	11.68	152	131571	4.04	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	80.80%


Target Compounds					Ovalue
25) Chloroform	4.44	83	40490	0.64 ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA V\DATA\VV051518\
Data File : VV005908.D
Acq On : 15 May 2018 11:34
Operator : SY/MD
Sample : J2658-11
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1


Quant Time: May 16 03:46:05 2018
Quant Method : W:\HPCHEM1\MSVOA V\METHOD\SOMVTR050518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed May 16 03:06:39 2018
Response via : Initial Calibration

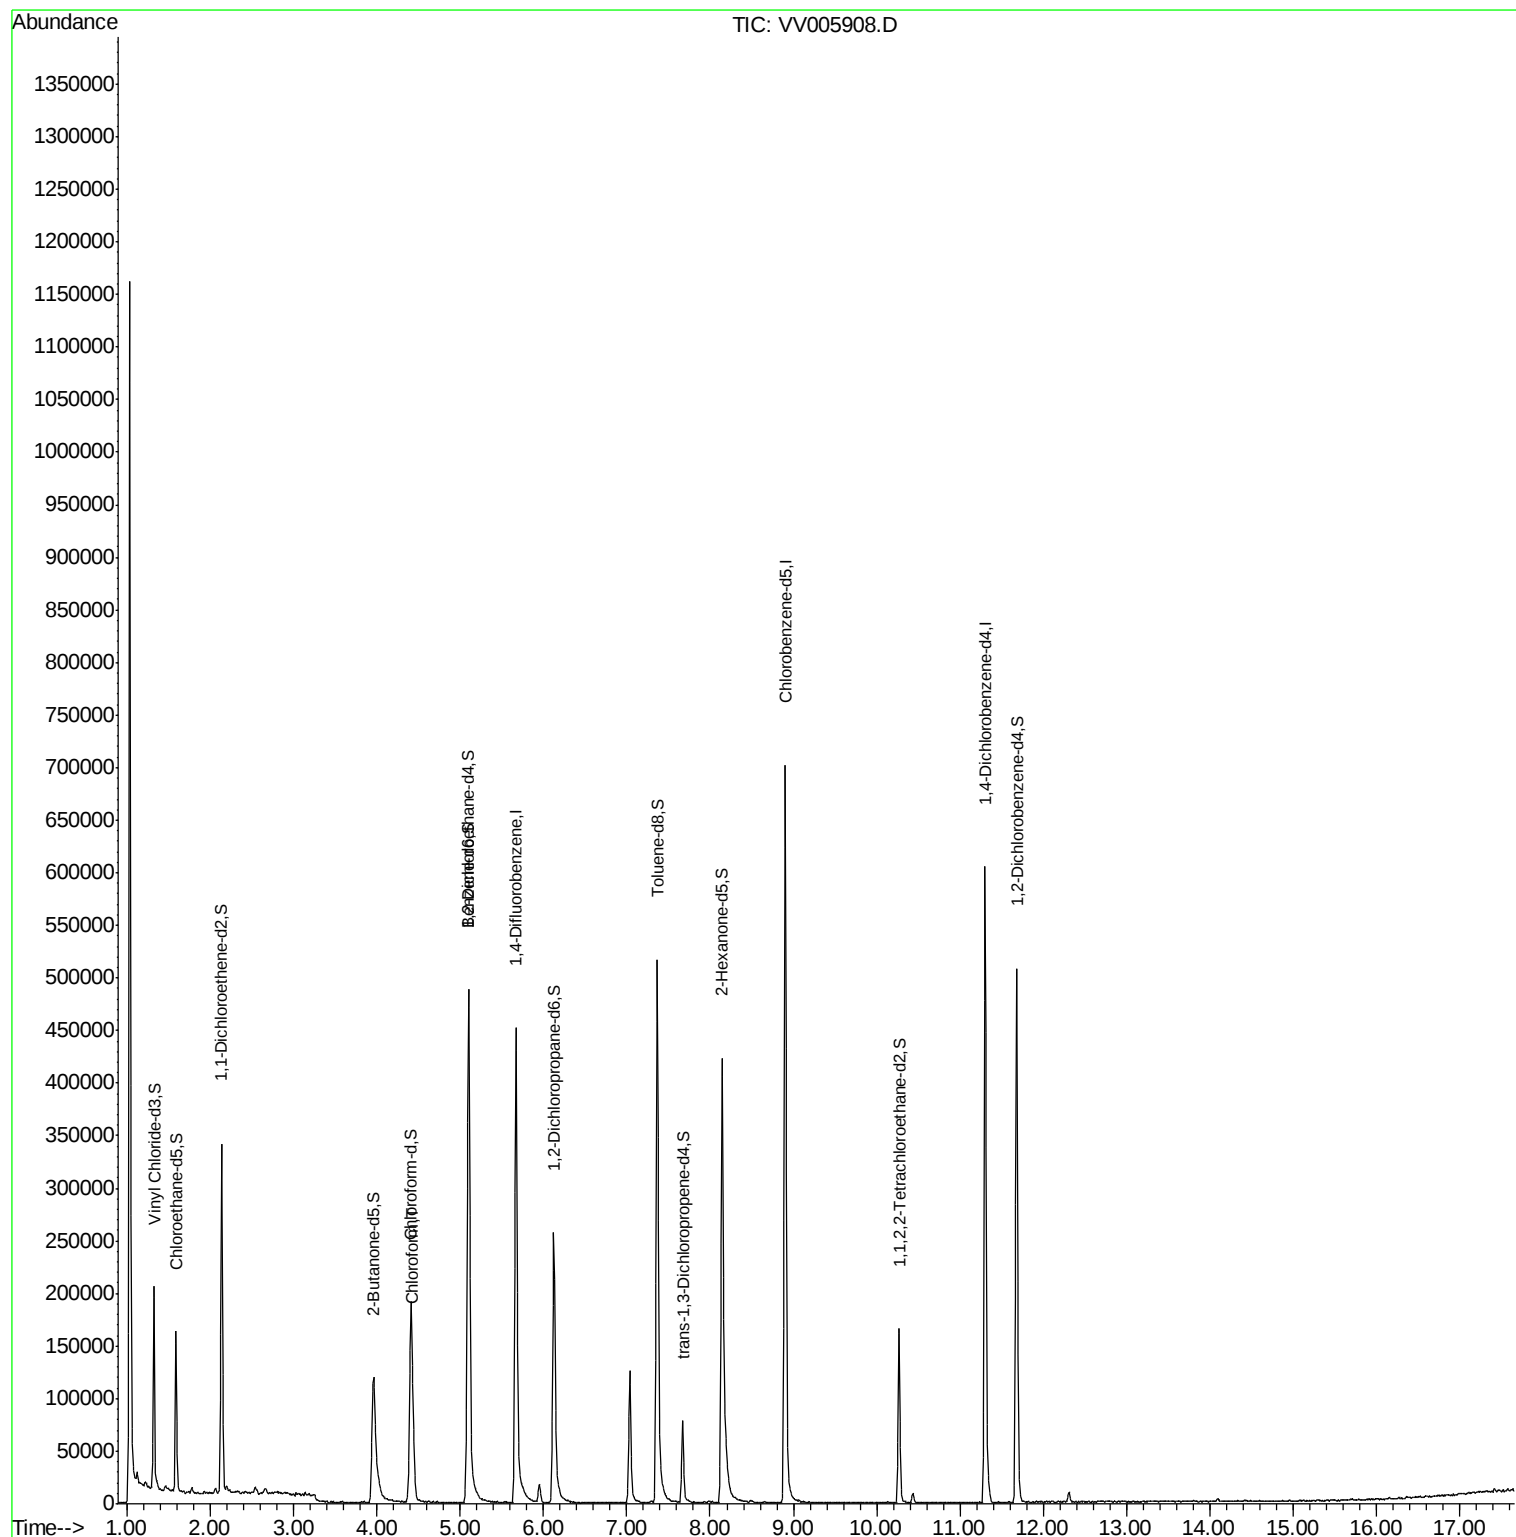

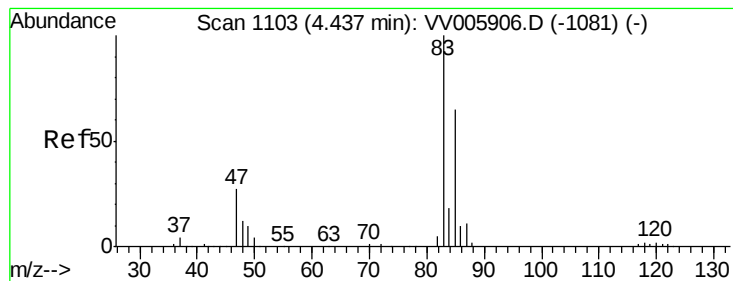

#25
 Chloroform
 Concen: 0.64 ug/L
 RT: 4.44 min Scan# 1103
 Delta R.T. -0.00 min
 Lab File: VV005908.D
 Acq: 15 May 2018 11:34

Tot Ion: 83 Resp: 40490
 Ion Ratio Lower Upper
 83 100
 85 61.5 47.1 87.5

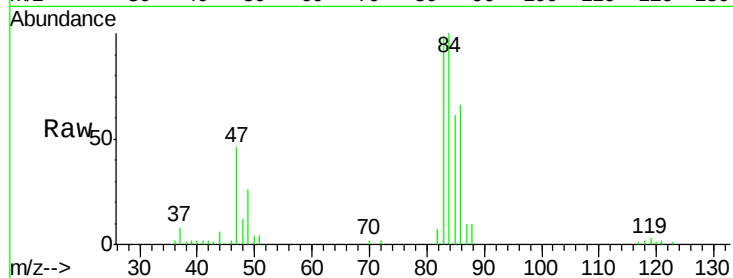

Abundance Ion 83.05 (82.75 to 83.75): VV0
 Ion 85.00 (84.70 to 85.70): VV0

