

Data Path : W:\HPCHEM1\MSVOA V\DATA\VV051518\
 Data File : VV005916.D
 Acq On : 15 May 2018 15:29
 Operator : SY/MD
 Sample : J2905-04
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 04:10:35 2018
 Quant Method : W:\HPCHEM1\MSVOA V\METHOD\SOMVTR050518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed May 16 03:06:39 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	279877	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	271975	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	110429	5.00	ug/L	0.00

System Monitoring Compounds


4) Vinyl Chloride-d3	1.32	65	89951	4.23	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.60%
7) Chloroethane-d5	1.58	69	82316	4.49	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.80%
11) 1,1-Dichloroethene-d2	2.13	63	137743	2.94	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	58.80%#
20) 2-Butanone-d5	3.96	46	234574	56.13	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	112.26%
24) Chloroform-d	4.41	84	205467	5.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.00%
26) 1,2-Dichloroethane-d4	5.09	65	109917	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.80%
32) Benzene-d6	5.11	84	379340	5.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.80%
36) 1,2-Dichloropropane-d6	6.13	67	120403	5.31	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.20%
41) Toluene-d8	7.37	98	318857	4.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.40%
43) trans-1,3-Dichloropropene-	7.67	79	37450	4.18	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.60%
46) 2-Hexanone-d5	8.14	63	140090	40.09	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.18%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	74271	4.36	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	129101	5.63	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	112.60%


Target Compounds					Ovalue
13) Acetone	2.20	43	18213	5.15 ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA V\DATA\VV051518\
Data File : VV005916.D
Acq On : 15 May 2018 15:29
Operator : SY/MD
Sample : J2905-04
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 04:10:35 2018
Quant Method : W:\HPCHEM1\MSVOA V\METHOD\SOMVTR050518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed May 16 03:06:39 2018
Response via : Initial Calibration

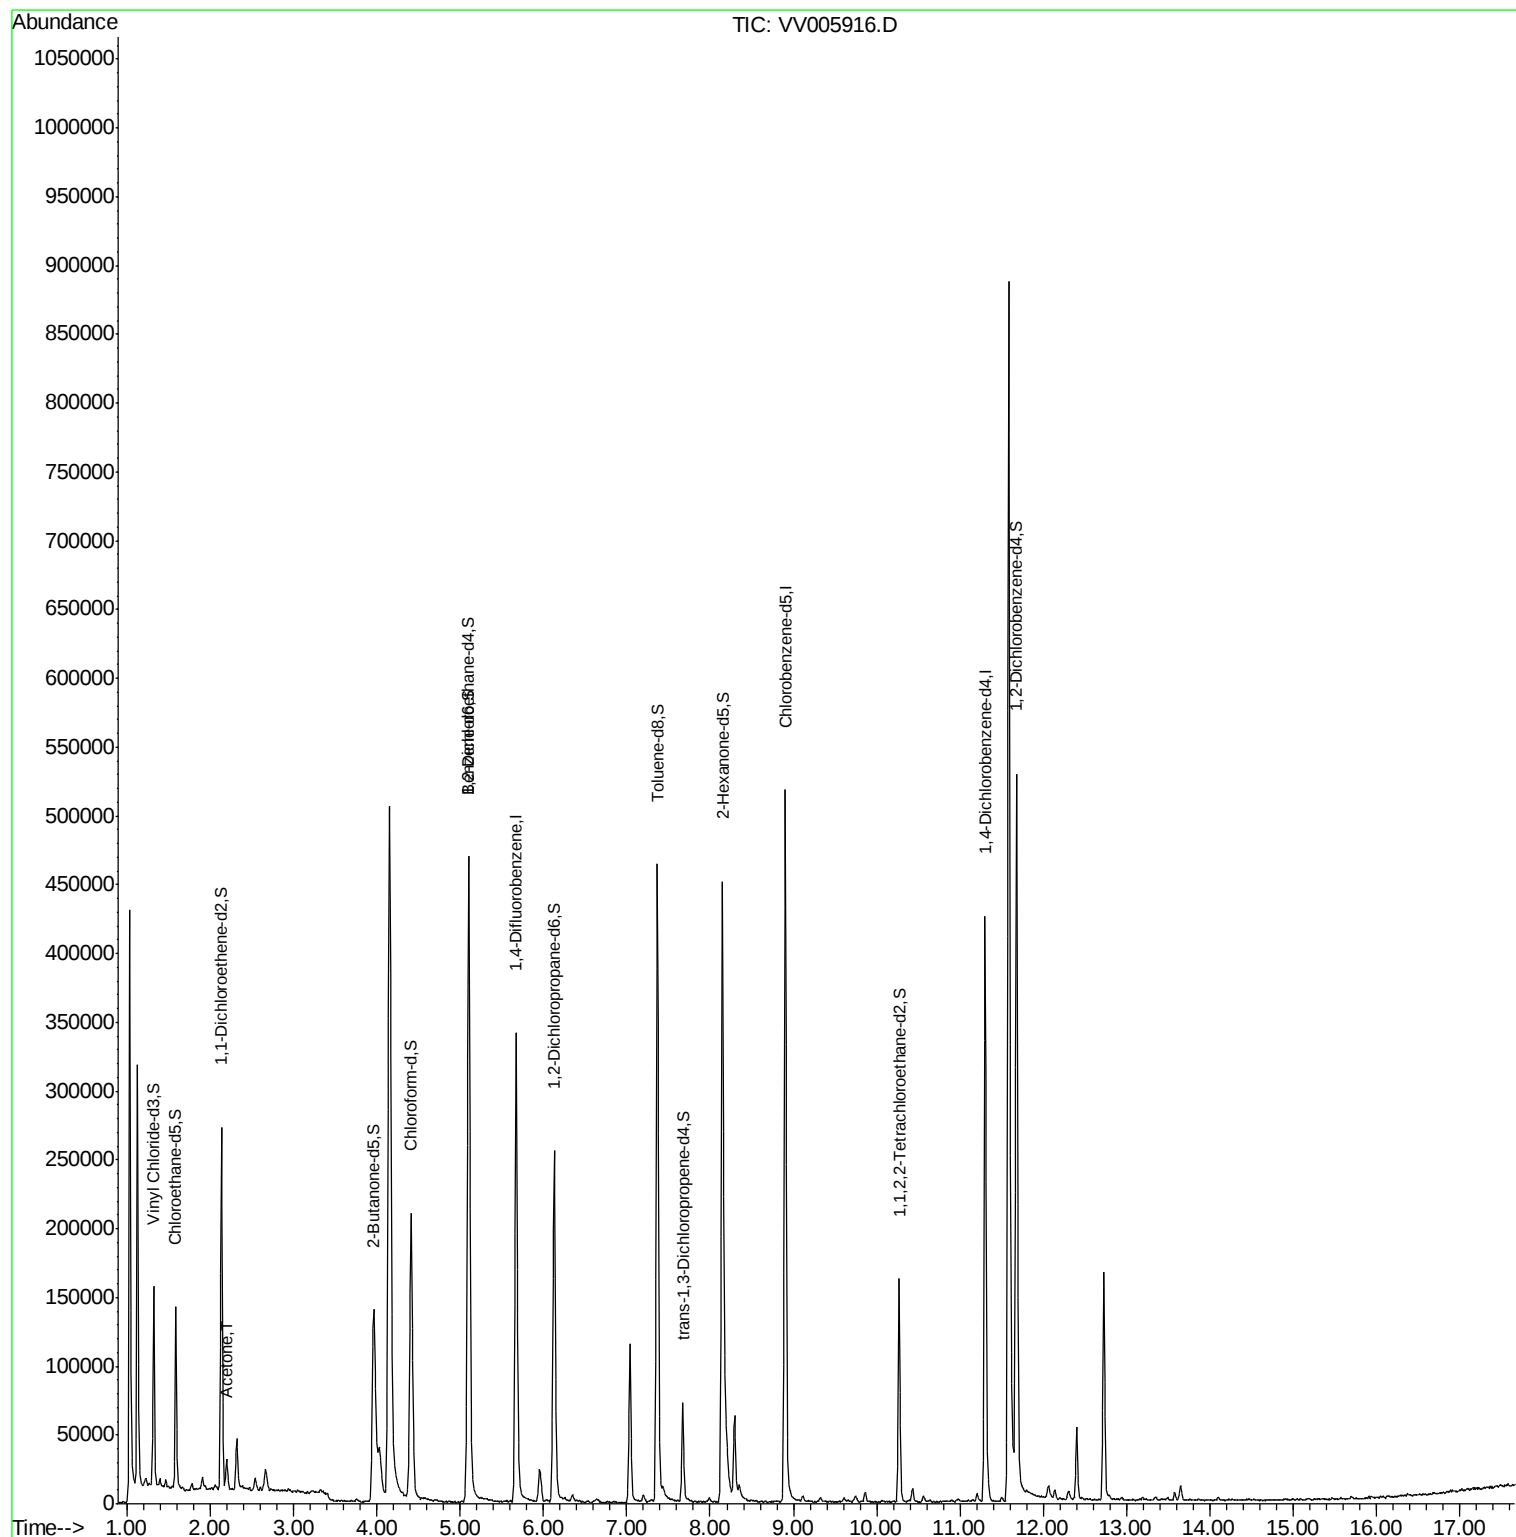

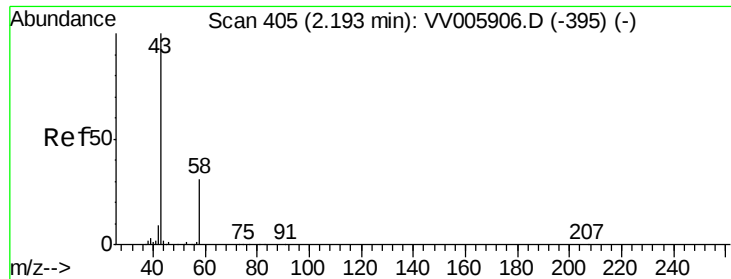

#13

Acetone

Concen: 5.15 ug/L

RT: 2.20 min Scan# 406

Delta R.T. 0.00 min

Lab File: VV005916.D

Acq: 15 May 2018 15:29

Tot Ion: 43 Resp: 18213

Ion Ratio Lower Upper

43 100

58 33.4 0.0 57.8

