


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV051520\
Data File : VV016085.D
Acq On : 15 May 2020 13:34
Operator : SY/MD
Sample : L2661-07
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4205

Manual Integrations
APPROVED

apatel
5/19/2020 2:01:09 PM

Quant Time: May 16 02:24:32 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat May 16 01:43:07 2020
Response via : Initial Calibration

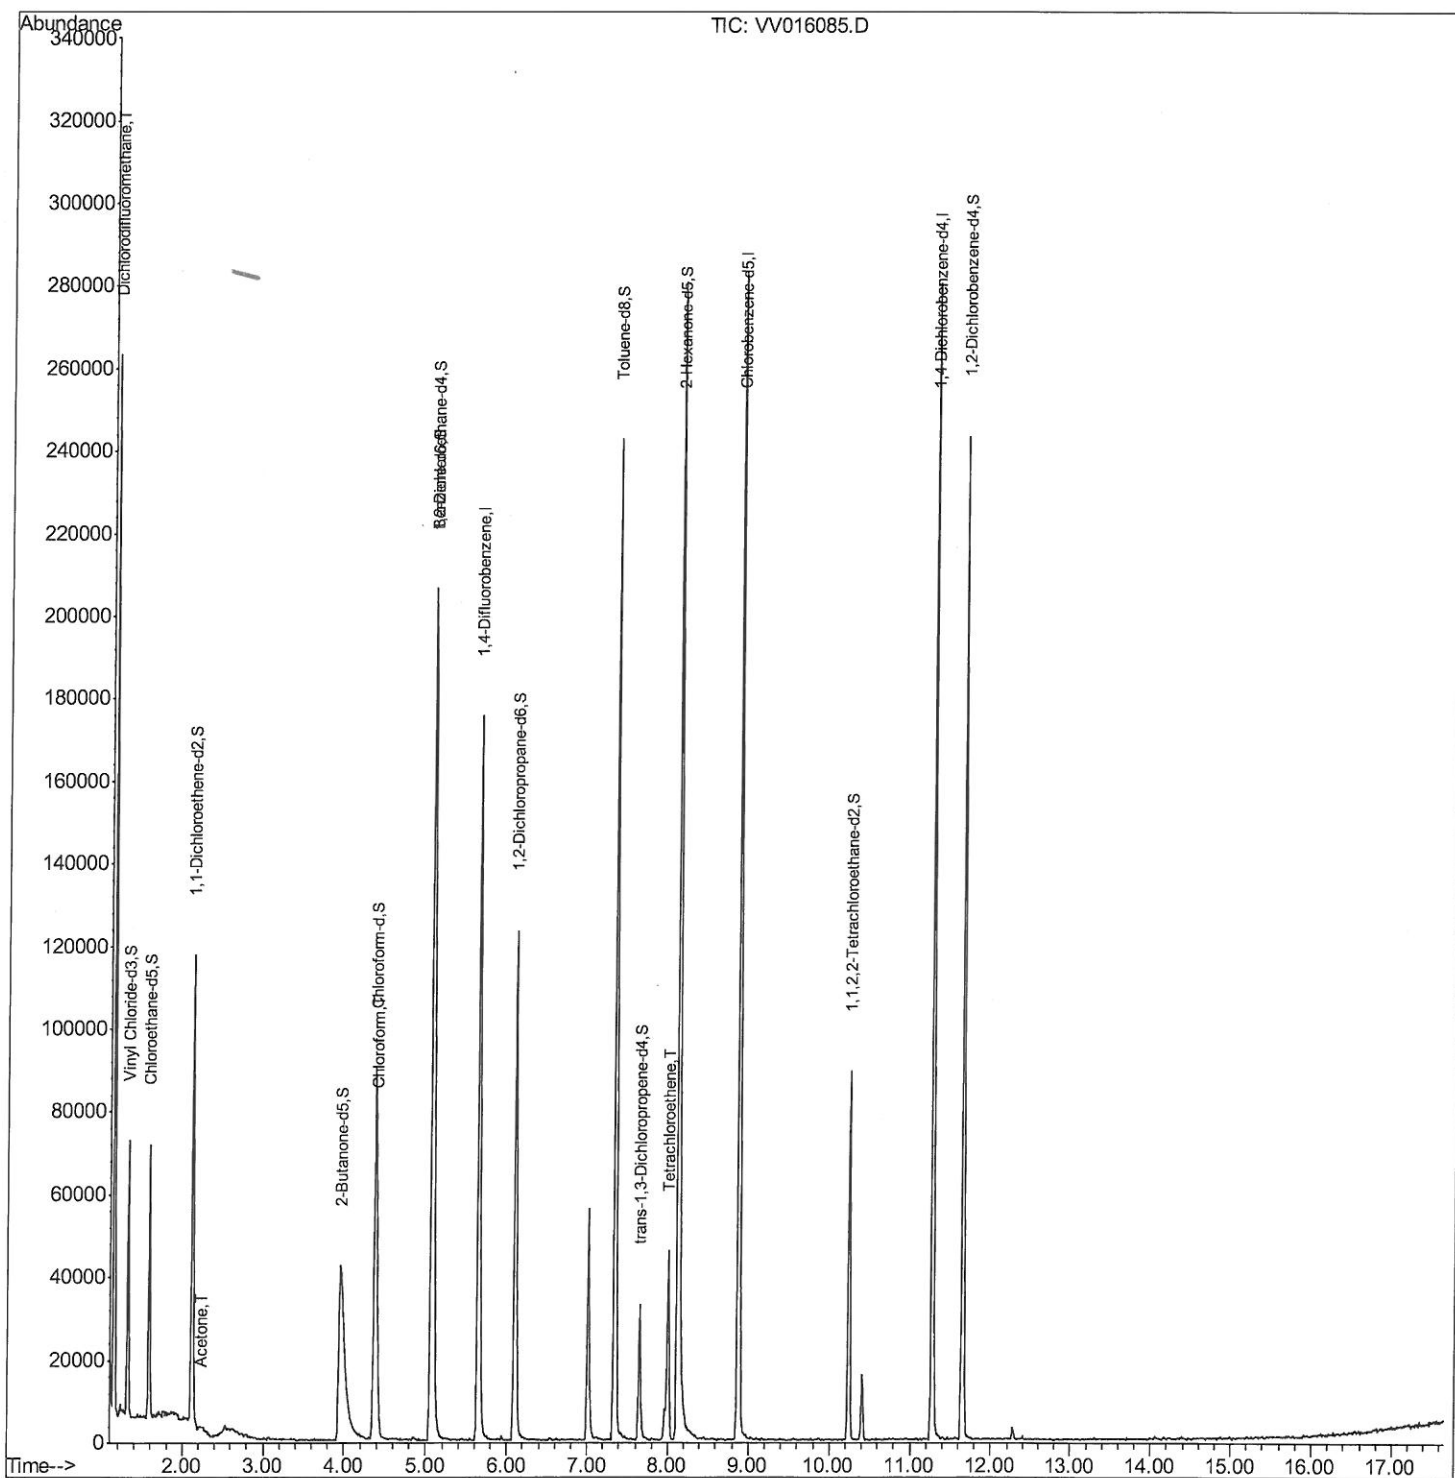

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV051520\
 Data File : VV016085.D
 Acq On : 15 May 2020 13:34
 Operator : SY/MD
 Sample : L2661-07
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4205

Manual Integrations
 APPROVED

apatel
 5/19/2020 2:01:09 PM

Quant Time: May 16 01:45:31 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 16 01:43:07 2020
 Response via : Initial Calibration

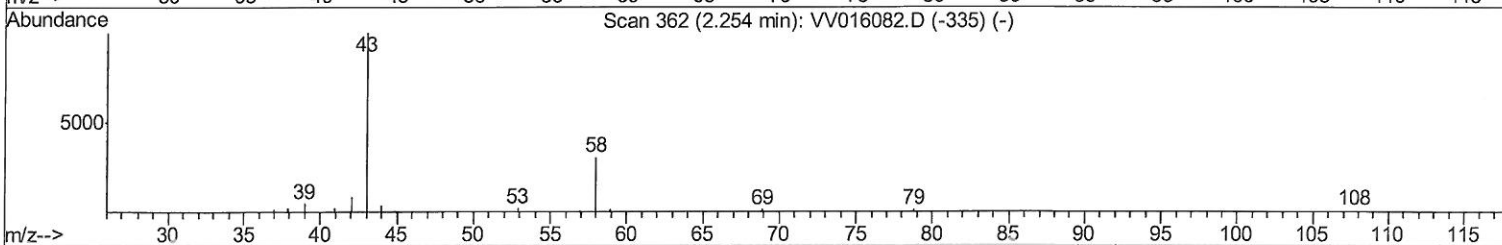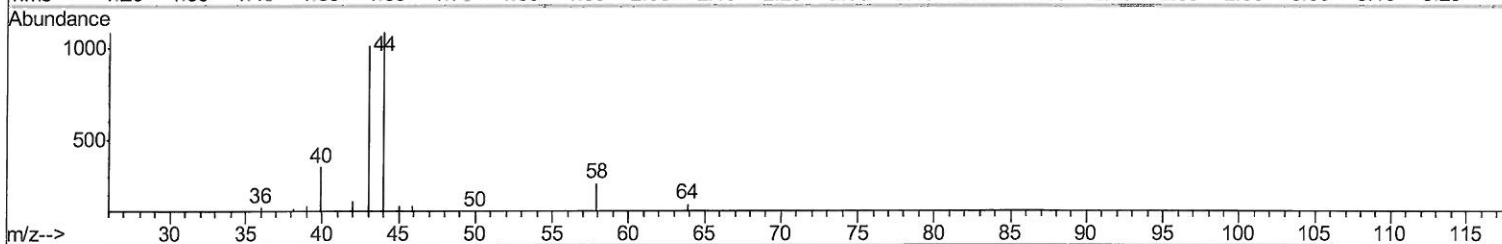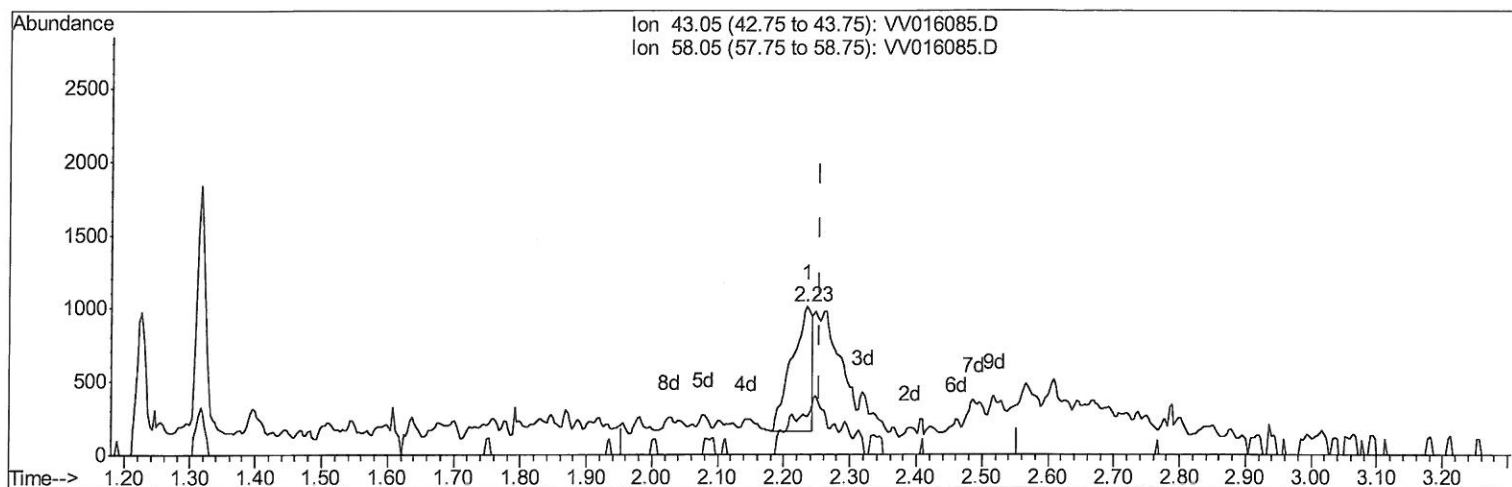

TIC: VV016085.D

(13) Acetone (T)

2.235min (-0.019) 1.22ug/L

response 1747

Ion	Exp%	Act%
43.05	100	100
58.05	15.40	14.54
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV051520\
 Data File : VV016085.D
 Acq On : 15 May 2020 13:34
 Operator : SY/MD
 Sample : L2661-07
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4205

Manual Integrations
 APPROVED

apatel
 5/19/2020 2:01:09 PM

Quant Time: May 16 01:45:31 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 16 01:43:07 2020
 Response via : Initial Calibration

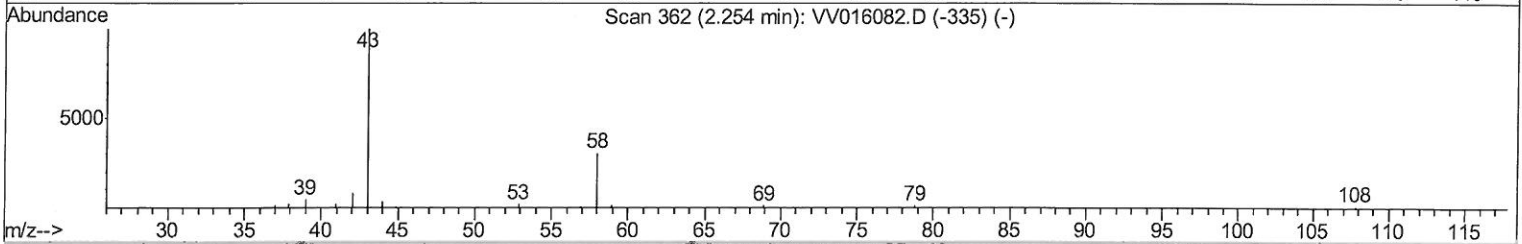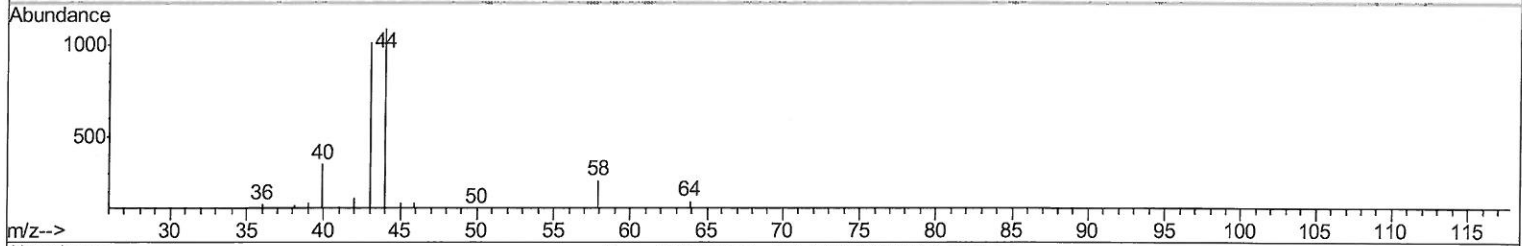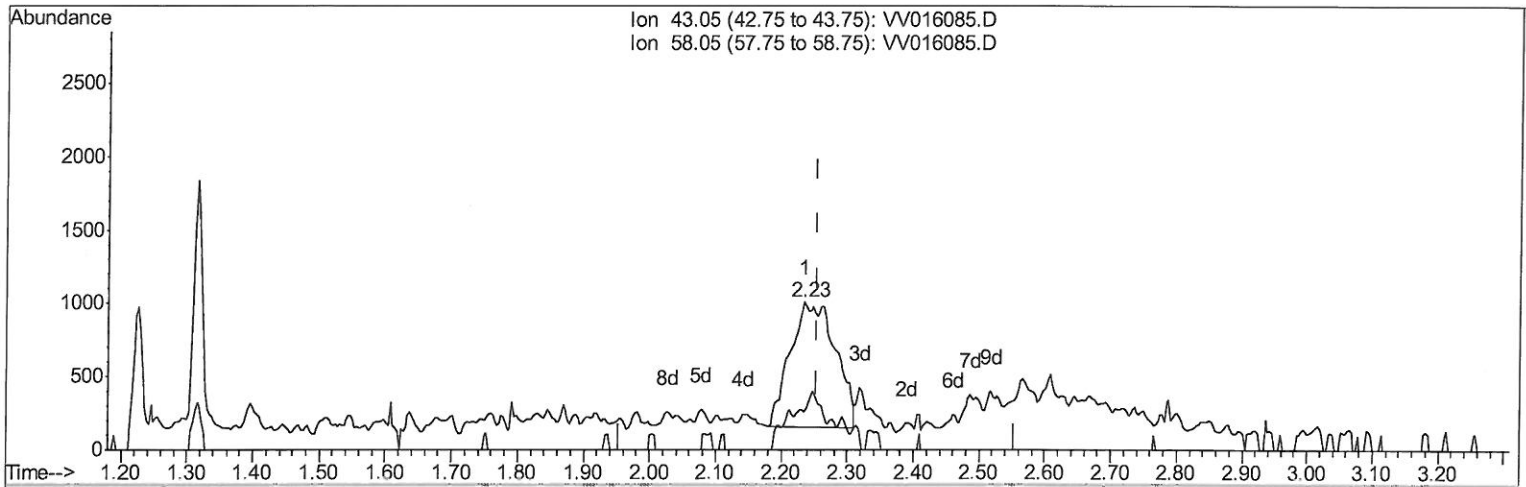

TIC: VV016085.D

(13) Acetone (T)

2.235min (-0.019) 2.84ug/L m

response 4067

Ion	Exp%	Act%
43.05	100	100
58.05	15.40	6.25
0.00	0.00	0.00
0.00	0.00	0.00

MD
 5/22/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV051520\
 Data File : VV016085.D
 Acq On : 15 May 2020 13:34
 Operator : SY/MD
 Sample : L2661-07
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampled :
 H4205

Manual Integrations
 APPROVED

apatel
 5/19/2020 2:01:09 PM

Quant Time: May 16 02:24:32 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 16 01:43:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	5.64	114	140187	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	141969	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	65131	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.32	65	38144	5.02	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	100.40%		
7) Chloroethane-d5	1.58	69	40306	5.59	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	111.80%		
11) 1,1-Dichloroethene-d2	2.12	63	61173	3.74	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	74.80%		
20) 2-Butanone-d5	3.95	46	128552	59.26	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	118.52%		
24) Chloroform-d	4.38	84	88587	5.33	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	106.60%		
26) 1,2-Dichloroethane-d4	5.06	65	51582	5.41	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	108.20%		
32) Benzene-d6	5.08	84	172361	5.10	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	102.00%		
36) 1,2-Dichloropropane-d6	6.10	67	54928	5.33	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	106.60%		
41) Toluene-d8	7.34	98	149490	4.68	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	93.60%		
45) trans-1,3-Dichloropropene-	7.65	79	18099	4.47	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	89.40%		
48) 2-Hexanone-d5	8.12	63	99128	55.76	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	111.52%		
59) 1,1,2,2-Tetrachloroethane-	10.24	84	40951	5.65	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	113.00%		
65) 1,2-Dichlorobenzene-d4	11.65	152	56995	5.39	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	107.80%		
Target Compounds						
2) Dichlorodifluoromethane	1.14	85	2790	0.260	ug/L	96
13) Acetone	2.23	43	4067m	2.842	ug/L	
25) Chloroform	4.40	83	7061	0.390	ug/L	92
49) Tetrachloroethene	8.00	164	9719	1.366	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

2 m8
 5/22/20