


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV051520\
Data File : VV016081.D
Acq On : 15 May 2020 09:26
Operator : SY/MD
Sample : BFB58
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB58

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050720WMA.M
Title : TRACE VOA SOM01.0
Last Update : Sat May 16 01:43:07 2020

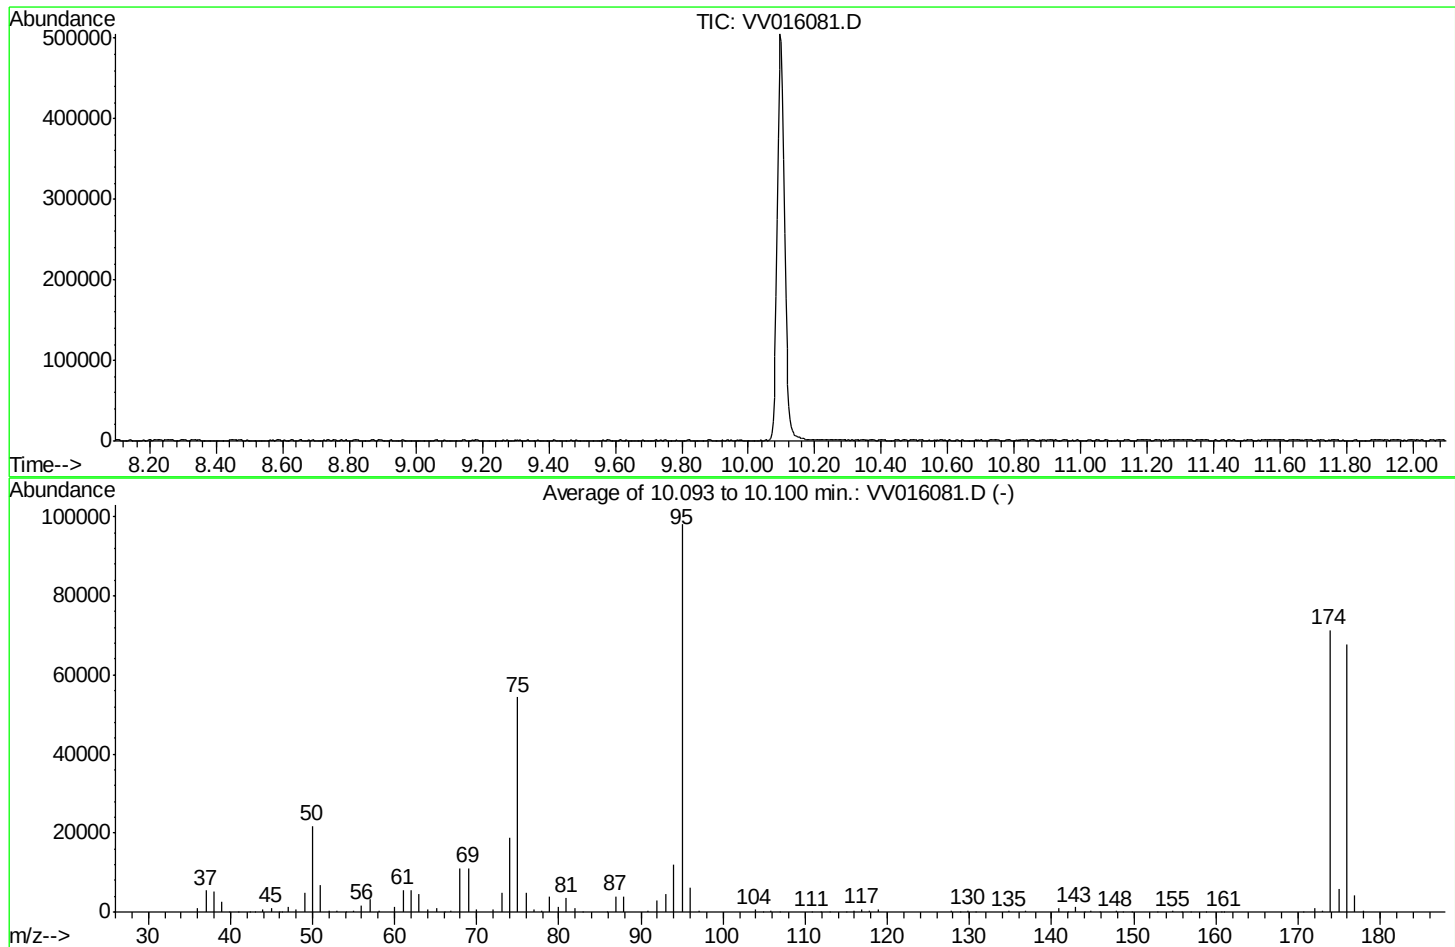

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	21800	PASS
75	95	30	80	55.4	54357	PASS
95	95	100	100	100.0	98114	PASS
96	95	5	9	6.4	6281	PASS
173	174	0.00	2	0.5	324	PASS
174	95	50	120	72.7	71301	PASS
175	174	5	9	8.0	5681	PASS
176	174	95	101	95.1	67837	PASS
177	176	5	9	6.3	4281	PASS

m/z	Abundance
36.00	1121.0
37.00	5135.0
38.00	5066.0
39.00	2390.0
39.90	370.0
42.30	105.0
43.00	134.0
44.00	1022.0
45.00	1090.0
45.90	223.0
47.00	1203.0
48.00	621.0
49.00	4754.0
50.00	20888.0
51.00	6266.0
52.00	430.0
52.90	193.0
55.00	296.0
56.00	1657.0
57.00	3215.0
58.10	169.0
59.90	1137.0
61.00	5574.0
62.00	5284.0
63.00	4269.0
63.90	510.0
65.10	790.0
66.80	304.0
68.00	10395.0
69.00	10750.0
69.90	701.0
71.90	534.0
73.00	4513.0
74.00	18112.0
75.00	51896.0
76.00	4845.0
76.90	564.0
77.90	346.0
78.90	3862.0
79.90	1196.0
80.90	3522.0
81.90	827.0
82.90	124.0
85.90	202.0
86.90	3709.0
88.00	3694.0
90.90	404.0
92.00	2747.0
93.00	4356.0
94.00	11659.0
95.00	92808.0
96.00	6059.0
97.00	209.0
103.90	465.0
104.90	136.0
105.80	414.0
106.90	113.0
110.80	154.0
112.90	135.0
115.00	142.0
115.90	393.0
116.90	690.0
117.80	444.0
118.90	647.0
127.80	319.0
128.80	142.0
129.80	365.0
130.80	132.0
134.90	225.0
136.70	220.0
140.80	1105.0
141.90	148.0
142.90	1145.0
144.80	207.0
145.90	133.0
147.90	226.0
148.70	122.0
149.70	102.0
153.00	107.0
154.80	220.0
156.90	169.0
158.80	138.0
160.70	103.0
161.10	111.0
170.60	112.0
172.00	1059.0
173.00	973.0
173.90	65544.0
175.00	5359.0
175.90	61944.0
176.90	4060.0
178.00	161.0

Instrument :
MSVOA_V
ClientSampleId :
BFB58

m/z	Abundance
36.00	1103.0
37.00	5557.0
38.00	5416.0
39.00	2571.0
40.00	393.0
43.00	148.0
44.00	1098.0
45.00	1172.0
45.90	174.0
47.00	1272.0
48.00	700.0
49.00	5043.0
50.00	22648.0
51.00	6926.0
52.00	467.0
52.90	225.0
54.00	104.0
55.00	370.0
56.00	1848.0
57.00	3482.0
58.00	191.0
59.90	1239.0
61.00	5841.0
62.00	5778.0
63.00	4606.0
63.90	529.0
65.10	942.0
66.80	395.0
68.00	11298.0
69.00	11584.0
70.00	801.0
71.90	570.0
73.00	4980.0
74.00	19512.0
75.00	56360.0
76.00	5124.0
76.90	645.0
77.90	362.0
78.90	4145.0
79.90	1202.0
80.90	3830.0
81.90	933.0
83.00	144.0
85.80	169.0
86.90	4159.0
87.90	3977.0
90.90	459.0
92.00	3083.0
93.00	4654.0
94.00	12497.0
95.00	101528.0
96.00	6486.0
97.00	208.0
103.90	519.0
104.90	159.0
105.80	476.0
110.80	179.0
111.80	102.0
112.90	140.0
114.90	156.0
115.90	468.0
116.90	784.0
117.80	442.0
118.90	719.0
127.80	409.0
128.80	145.0
129.90	402.0
130.80	143.0
134.90	255.0
136.70	240.0
140.90	1134.0
142.00	155.0
142.90	1287.0
143.90	128.0
144.80	256.0
145.80	136.0
147.80	222.0
148.70	106.0
149.70	135.0
153.00	111.0
154.70	280.0
155.90	111.0
156.80	156.0
158.70	113.0
161.00	135.0
170.60	116.0
172.00	1122.0
173.90	73936.0
175.00	5887.0
175.90	70344.0
177.00	4472.0
177.90	196.0

Instrument :
MSVOA_V
ClientSampleId :
BFB58

m/z	Abundance
36.00	1053.0
37.00	5514.0
38.00	5245.0
39.00	2403.0
40.00	398.0
41.00	129.0
43.00	145.0
44.00	1092.0
45.00	1115.0
45.80	126.0
46.20	108.0
47.00	1279.0
48.00	683.0
49.00	4797.0
50.00	21864.0
51.00	6776.0
52.00	397.0
53.00	210.0
54.90	436.0
56.00	1780.0
57.00	3321.0
58.00	173.0
59.90	1191.0
61.00	5562.0
62.00	5504.0
63.00	4421.0
64.00	521.0
65.10	906.0
66.10	119.0
66.90	400.0
68.00	10933.0
69.00	11157.0
70.00	838.0
71.90	594.0
73.00	4757.0
74.00	18560.0
75.00	54816.0
76.00	4719.0
76.90	636.0
77.90	409.0
78.90	3908.0
79.90	1086.0
80.90	3707.0
81.90	899.0
83.00	137.0
85.70	151.0
86.90	4065.0
87.90	3837.0
90.90	442.0
92.00	3128.0
93.00	4415.0
94.00	11952.0
95.00	100008.0
96.00	6298.0
97.00	180.0
103.90	545.0
104.90	178.0
105.80	514.0
110.80	176.0
111.90	112.0
112.90	124.0
114.90	165.0
115.90	467.0
116.90	728.0
117.80	447.0
118.90	702.0
127.80	423.0
128.80	148.0
129.90	411.0
130.80	150.0
134.70	238.0
136.80	196.0
140.90	1007.0
142.00	127.0
142.90	1270.0
144.00	134.0
144.80	264.0
145.90	139.0
147.80	221.0
149.70	135.0
152.80	107.0
154.80	308.0
155.90	104.0
156.80	171.0
161.00	142.0
172.00	1028.0
173.90	74424.0
175.00	5797.0
175.90	71224.0
177.00	4312.0
177.90	193.0

Instrument :
MSVOA_V
ClientSampleId :
BFB58

Scan 2788 (10.055 min): VV016081.D
BFB58

m/z	Abundance
39.90	362.0
43.90	521.0

Instrument :
MSVOA_V
ClientSampleId :
BFB58