
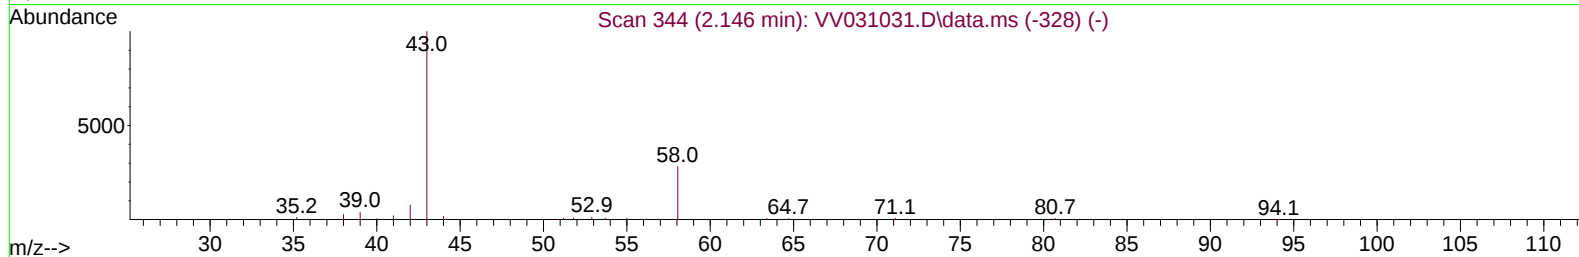
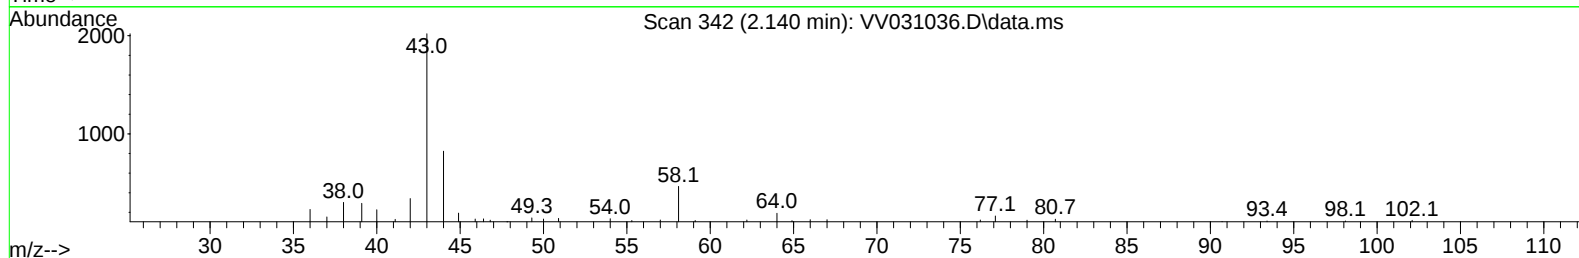


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051523\
 Data File : VV031036.D
 Acq On : 15 May 2023 19:22
 Operator : SY/MD
 Sample : 02768-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Quant Time: May 16 00:46:15 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue May 16 00:40:05 2023
 Response via : Initial Calibration

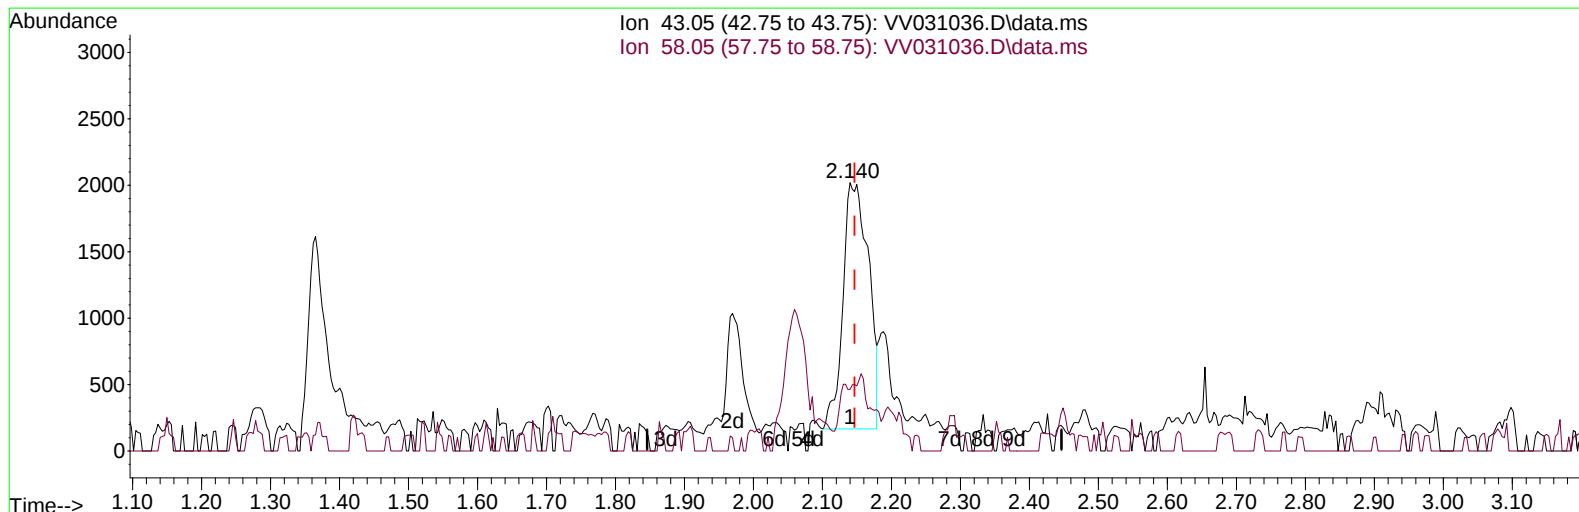

TIC: VV031036.D\data.ms

(13) Acetone (T)

2.140min (-0.006) 3.26 ug/L

response 4779

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	18.50	6.34
0.00	0.00	0.00
0.00	0.00	0.00