




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051523\
 Data File : VV031026.D
 Acq On : 15 May 2023 13:00
 Operator : SY/MD
 Sample : 02790-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CONY2

Manual IntegrationsAPPROVED

Quant Time: May 15 13:33:23 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat May 06 01:44:36 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/17/2023
 Supervised By :Mahesh Dadoda 05/17/2023

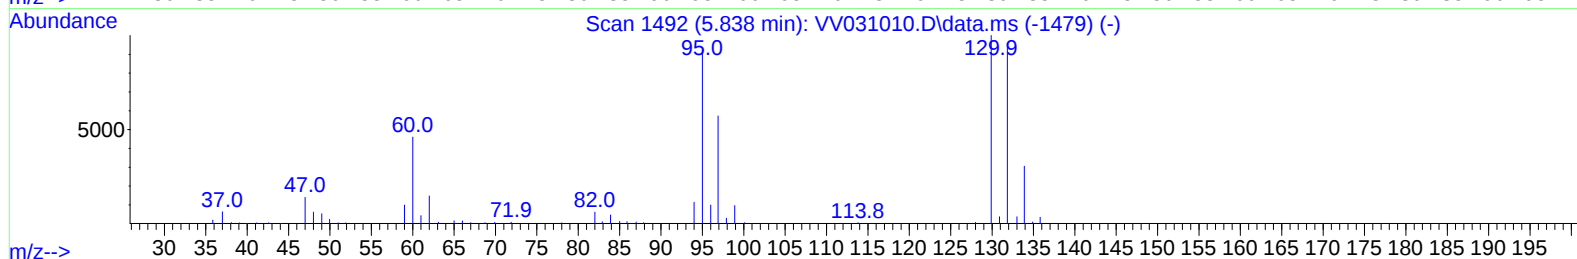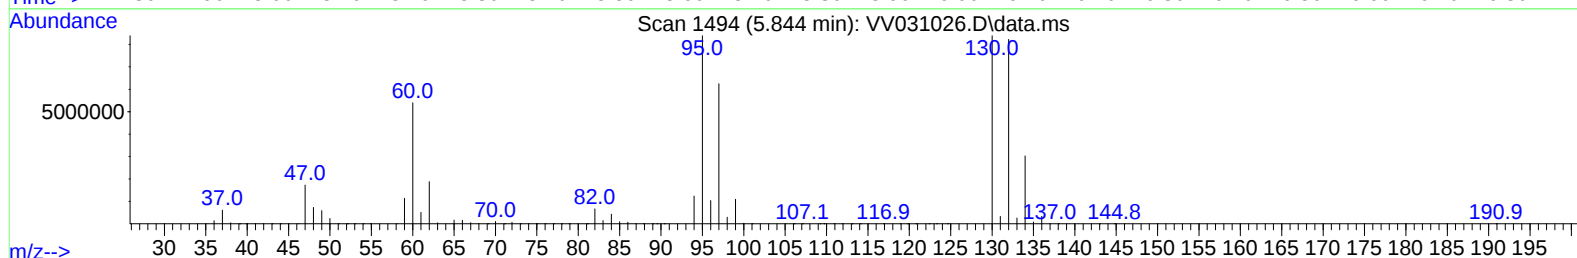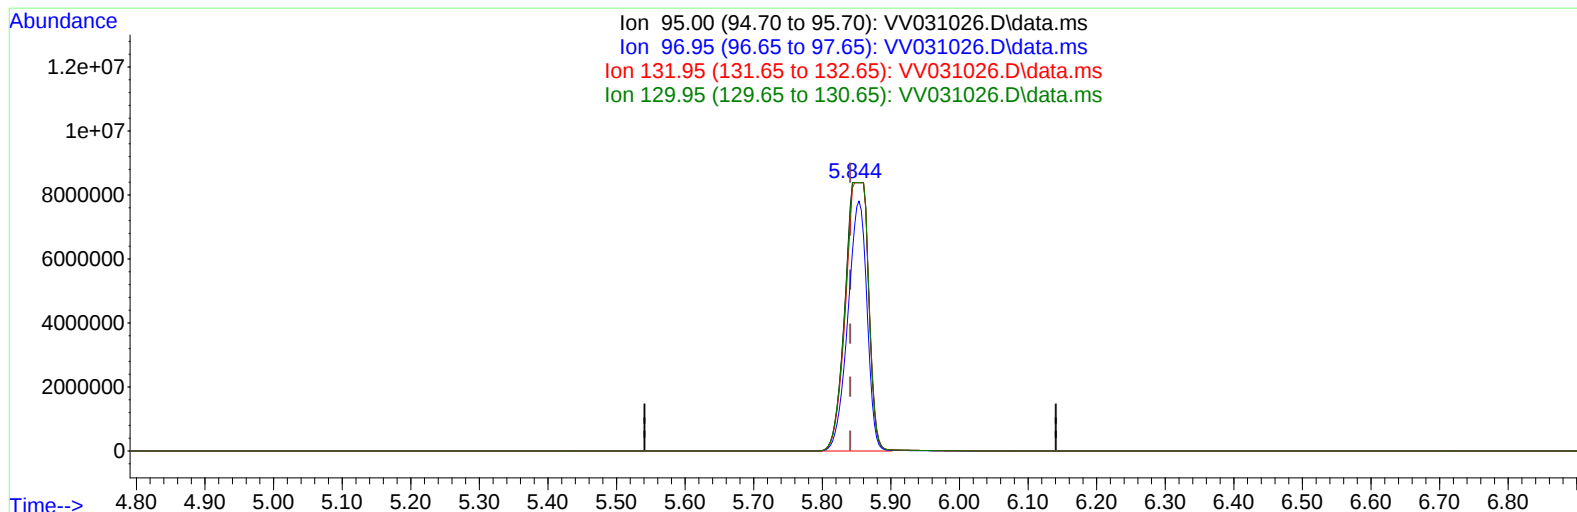

TIC: VV031026.D\data.ms

(34) Trichloroethene (T)

5.844min (+ 0.003) 2256.50 ug/L m

response 19942159

Ion	Exp%	Act%
95.00	100.00	100.00
96.95	66.00	74.48
131.95	103.90	98.05
129.95	108.10	100.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051523\
 Data File : VV031026.D
 Acq On : 15 May 2023 13:00
 Operator : SY/MD
 Sample : 02790-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CONY2

Manual IntegrationsAPPROVED

Quant Time: May 15 13:33:23 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat May 06 01:44:36 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/17/2023
 Supervised By :Mahesh Dadoda 05/17/2023

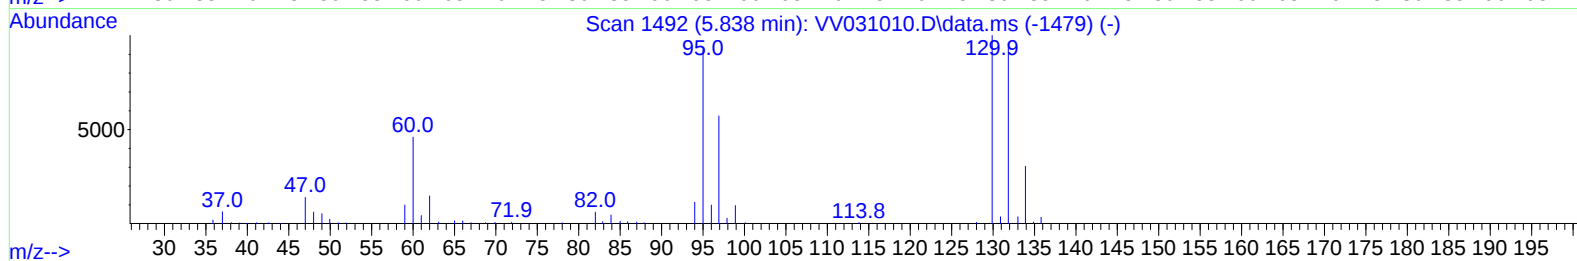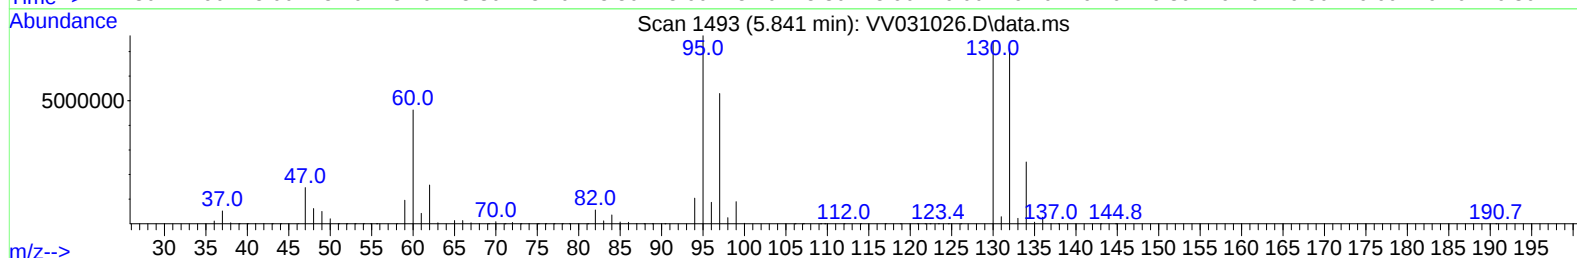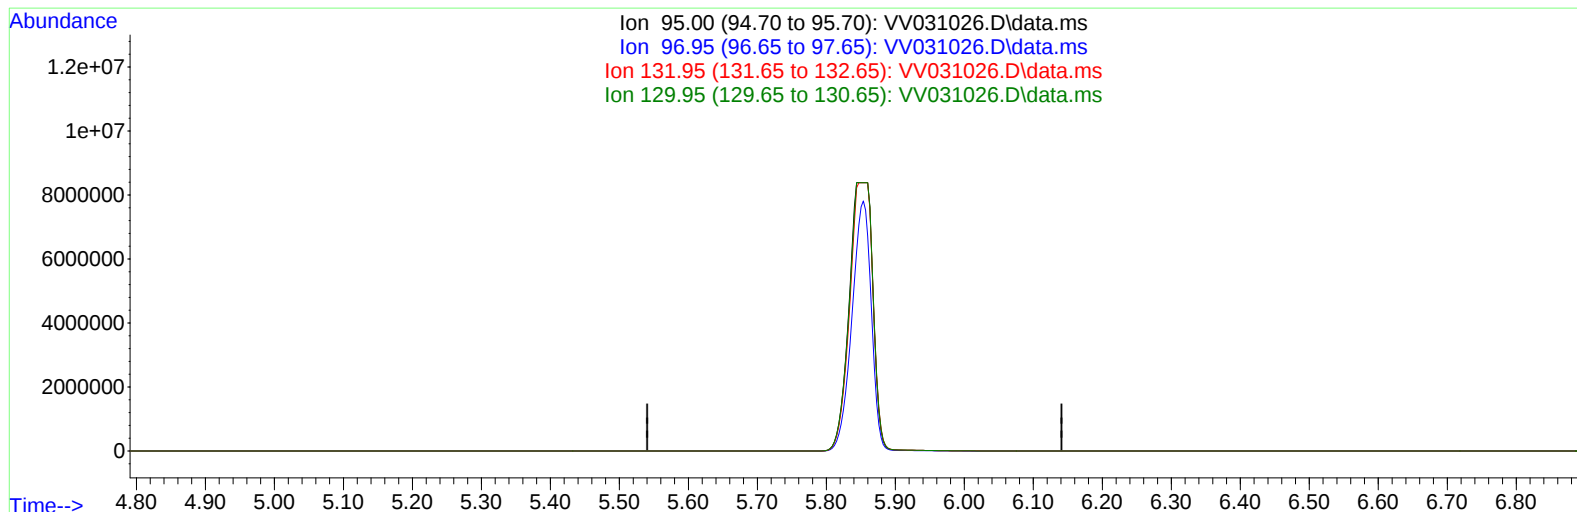

TIC: VV031026.D\data.ms

(34) Trichloroethene (T)

5.841min (-5.841) 0.00 ug/L

response 0

Ion	Exp%	Act%
95.00	100.00	0.00
96.95	66.00	0.00#
131.95	103.90	0.00#
129.95	108.10	0.00#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051523\
 Data File : VV031026.D
 Acq On : 15 May 2023 13:00
 Operator : SY/MD
 Sample : 02790-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CONY2

Manual IntegrationsAPPROVED

Quant Time: May 15 13:33:23 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat May 06 01:44:36 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/17/2023
 Supervised By :Mahesh Dadoda 05/17/2023

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	133865	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	131803	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	67680	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.285	65	55572	5.039	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 100.800%		
7) Chloroethane-d5	1.539	69	46145	5.129	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 102.600%		
11) 1,1-Dichloroethene-d2	2.066	65	26349	4.514	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 90.200%		
20) 2-Butanone-d5	3.815	46	136821	69.957	ug/L	-0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	= 139.920%#		
24) Chloroform-d	4.259	84	115864	5.286	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 105.800%		
26) 1,2-Dichloroethane-d4	4.953	65	59476	5.337	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 106.800%		
32) Benzene-d6	4.969	84	201368	5.212	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 104.200%		
36) 1,2-Dichloropropane-d6	5.998	67	62432	5.557	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 111.200%		
41) Toluene-d8	7.252	98	172581	4.691	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 93.800%		
43) trans-1,3-Dichloroprop...	7.561	79	20930	4.970	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 99.400%		
46) 2-Hexanone-d5	8.034	63	74265	50.335	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 100.680%		
56) 1,1,2,2-Tetrachloroeth...	10.159	84	40735	5.003	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 100.000%		
66) 1,2-Dichlorobenzene-d4	11.567	152	65125	5.162	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 103.200%		
Target Compounds						
						Qvalue
3) Chloromethane	1.217	50	3090	0.249	ug/L	98
5) Vinyl chloride	1.288	62	747327	71.948	ug/L	99
8) Chloroethane	1.555	64	13543	2.142	ug/L	99
12) 1,1-Dichloroethene	2.076	96	106332	11.803	ug/L #	73
13) Acetone	2.150	43	4704	2.816	ug/L	91
18) trans-1,2-Dichloroethene	2.703	96	127847	15.536	ug/L	97
19) 1,1-Dichloroethane	3.127	63	4881	0.307	ug/L	95
22) cis-1,2-Dichloroethene	3.821	96	6020314	693.404	ug/L	93
29) 1,1,1-Trichloroethane	4.522	97	16095	0.972	ug/L	97
34) Trichloroethene	5.844	95	19942159m	2256.497	ug/L	
42) Toluene	7.323	91	111636	3.128	ug/L	98
47) Tetrachloroethene	7.918	164	1394	0.165	ug/L	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051523\
Data File : VV031026.D
Acq On : 15 May 2023 13:00
Operator : SY/MD
Sample : 02790-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONY2

Manual IntegrationsAPPROVED

Quant Time: May 15 13:33:23 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat May 06 01:44:36 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 05/17/2023
Supervised By :Mahesh Dadoda 05/17/2023

