

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW051523\
 Data File : VW031020.D
 Acq On : 15 May 2023 10:36
 Operator : SY/MD
 Sample : 02790-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CONX6

Quant Time: May 15 12:16:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat May 06 01:44:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	141118	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	137295	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	70571	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	43235	3.719	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	74.400%
7) Chloroethane-d5	1.539	69	41282	4.353	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.000%
11) 1,1-Dichloroethene-d2	2.066	65	23677	3.848	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.000%
20) 2-Butanone-d5	3.818	46	86959	42.177	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	84.360%
24) Chloroform-d	4.259	84	99699	4.315	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.200%
26) 1,2-Dichloroethane-d4	4.953	65	51740	4.405	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.000%
32) Benzene-d6	4.970	84	170106	4.227	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.600%
36) 1,2-Dichloropropane-d6	5.998	67	49025	4.189	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	83.800%
41) Toluene-d8	7.252	98	145307	3.792	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.800%
43) trans-1,3-Dichloroprop...	7.564	79	17651	4.024	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.400%
46) 2-Hexanone-d5	8.034	63	57814	37.618	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	75.240%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	34918	4.117	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	82.400%
66) 1,2-Dichlorobenzene-d4	11.567	152	56902	4.326	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	86.600%
Target Compounds						Qvalue
34) Trichloroethene	5.844	95	5252	0.571	ug/L	91
42) Toluene	7.323	91	45129	1.214	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051523\
Data File : VV031020.D
Acq On : 15 May 2023 10:36
Operator : SY/MD
Sample : 02790-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONX6

Quant Time: May 15 12:16:38 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat May 06 01:44:36 2023
Response via : Initial Calibration




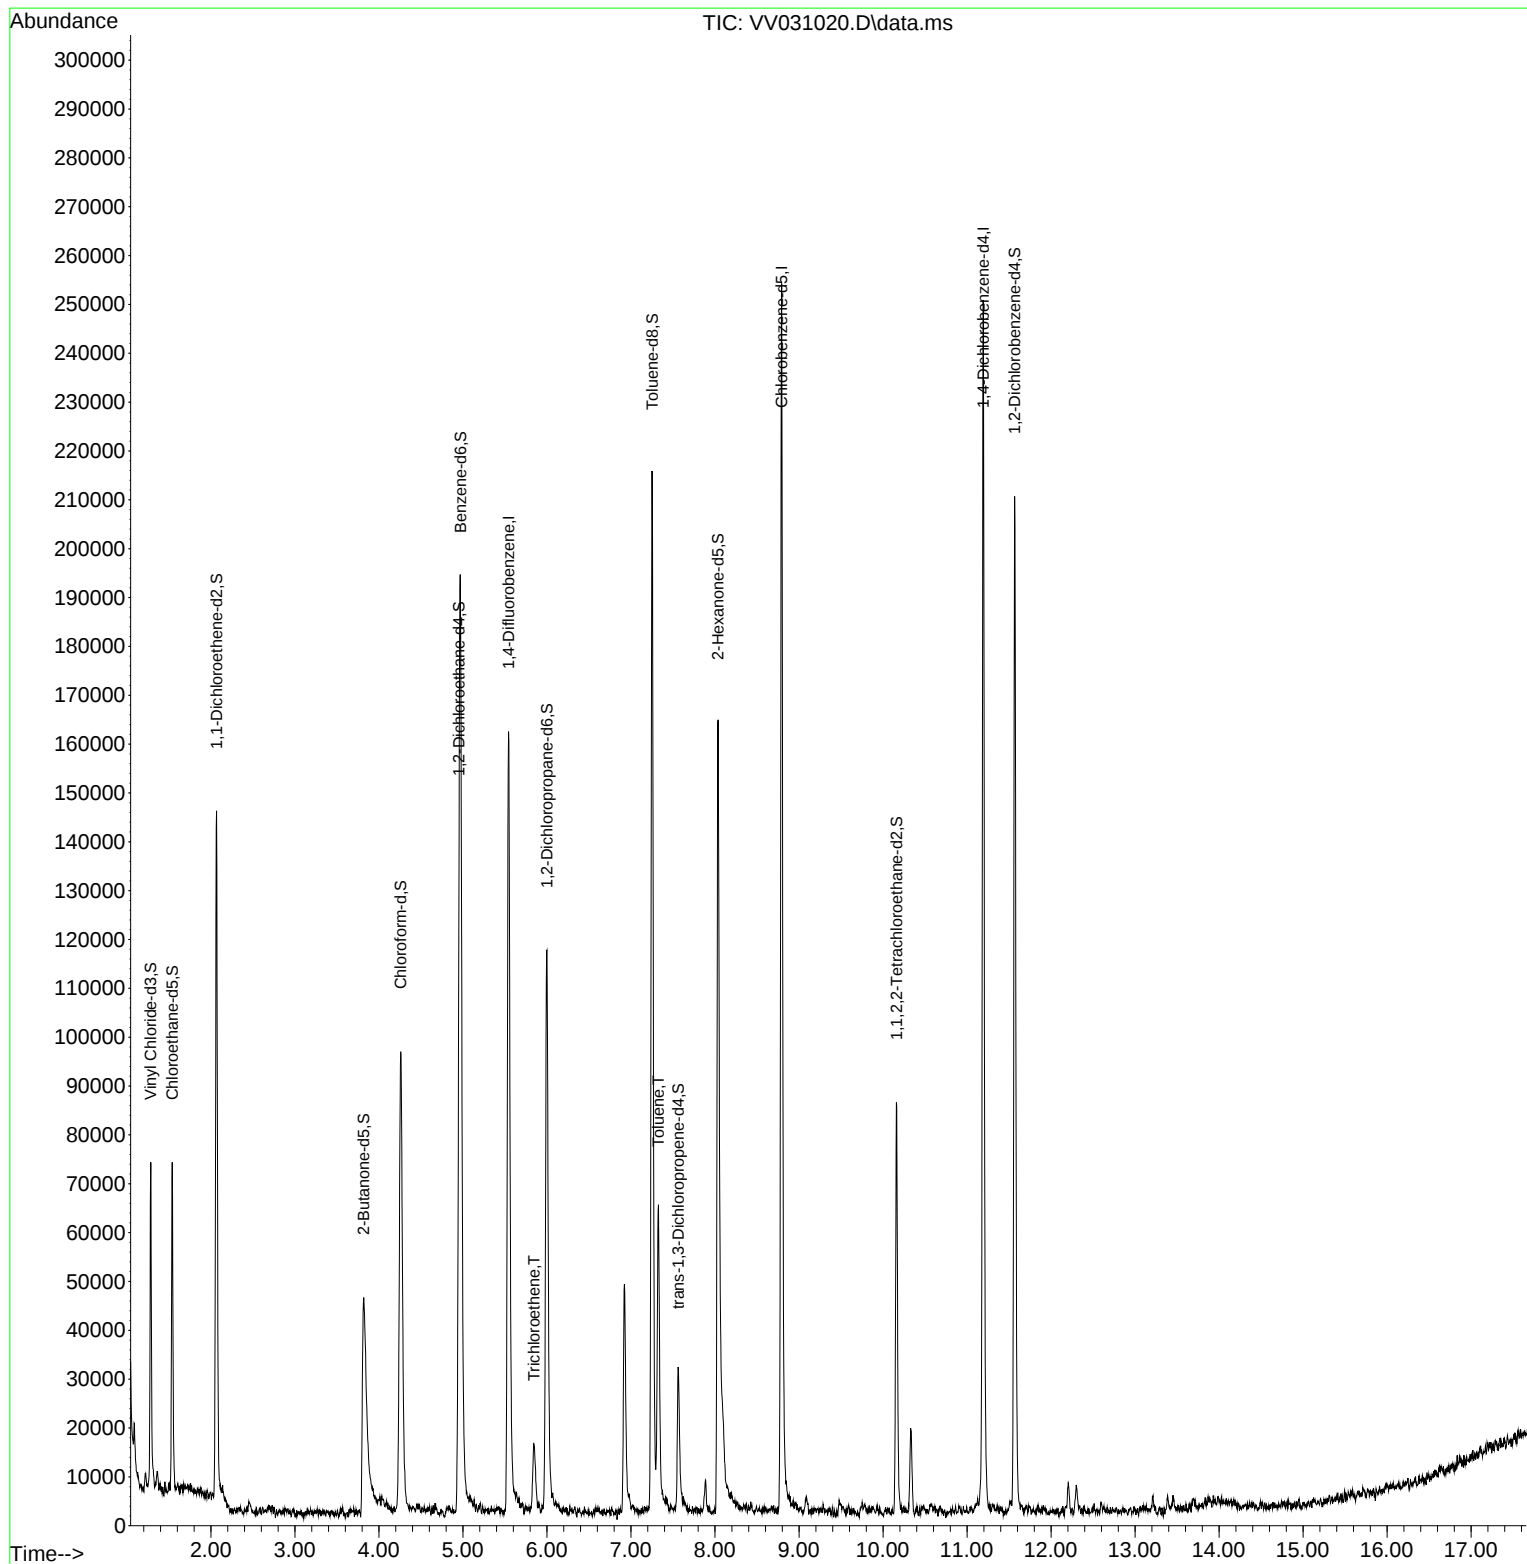


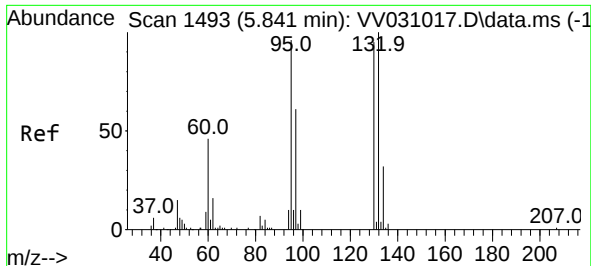

#34
Trichloroethene
Concen: 0.571 ug/L
RT: 5.844 min Scan# 1493
Delta R.T. 0.003 min
Lab File: VV031020.D
Acq: 15 May 2023 10:36

Instrument :
MSVOA_V
ClientSampleId :
CONX6

Tgt Ion:	95	Resp:	5252
Ion	Ratio	Lower	Upper
95	100		
97	65.6	46.2	85.8
132	92.5	72.7	135.1
130	95.2	75.7	140.5

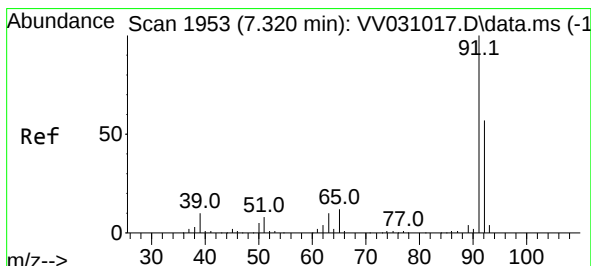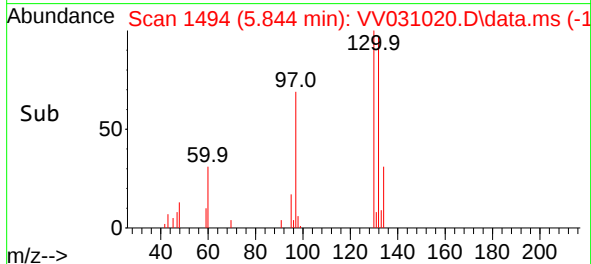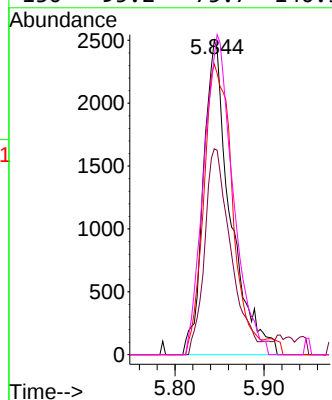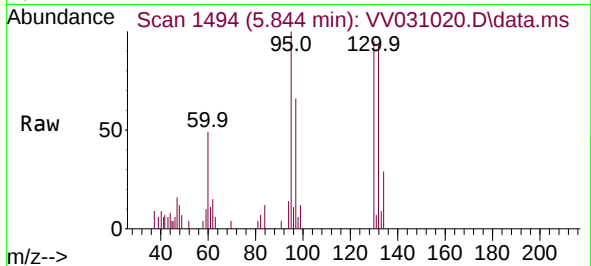

#42
Toluene
Concen: 1.214 ug/L
RT: 7.323 min Scan# 1954
Delta R.T. 0.000 min
Lab File: VV031020.D
Acq: 15 May 2023 10:36

Tgt Ion:	91	Resp:	45129
Ion	Ratio	Lower	Upper
91	100		
92	59.2	40.5	75.1

