

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW051523\
 Data File : VW031029.D
 Acq On : 15 May 2023 16:29
 Operator : SY/MD
 Sample : 02768-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CONP3

Quant Time: May 16 00:16:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue May 16 00:10:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	123253	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	122538	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	62471	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	46414	4.571	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.400%
7) Chloroethane-d5	1.536	69	44627	5.387	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	107.800%
11) 1,1-Dichloroethene-d2	2.063	65	24307	4.523	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	90.400%
20) 2-Butanone-d5	3.818	46	106783	59.299	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	118.600%
24) Chloroform-d	4.259	84	106945	5.299	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.000%
26) 1,2-Dichloroethane-d4	4.953	65	57491	5.603	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.000%
32) Benzene-d6	4.969	84	182480	5.080	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.600%
36) 1,2-Dichloropropane-d6	5.995	67	55691	5.332	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.600%
41) Toluene-d8	7.249	98	155958	4.560	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.200%
43) trans-1,3-Dichloroprop...	7.561	79	19014	4.857	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	97.200%
46) 2-Hexanone-d5	8.034	63	71268	51.956	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.920%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	40902	5.403	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.000%
66) 1,2-Dichlorobenzene-d4	11.567	152	62177	5.339	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.800%
Target Compounds						
					Qvalue	
34) Trichloroethene	5.850	95	3591	0.437	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051523\
Data File : VV031029.D
Acq On : 15 May 2023 16:29
Operator : SY/MD
Sample : 02768-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONP3


Quant Time: May 16 00:16:24 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue May 16 00:10:06 2023
Response via : Initial Calibration

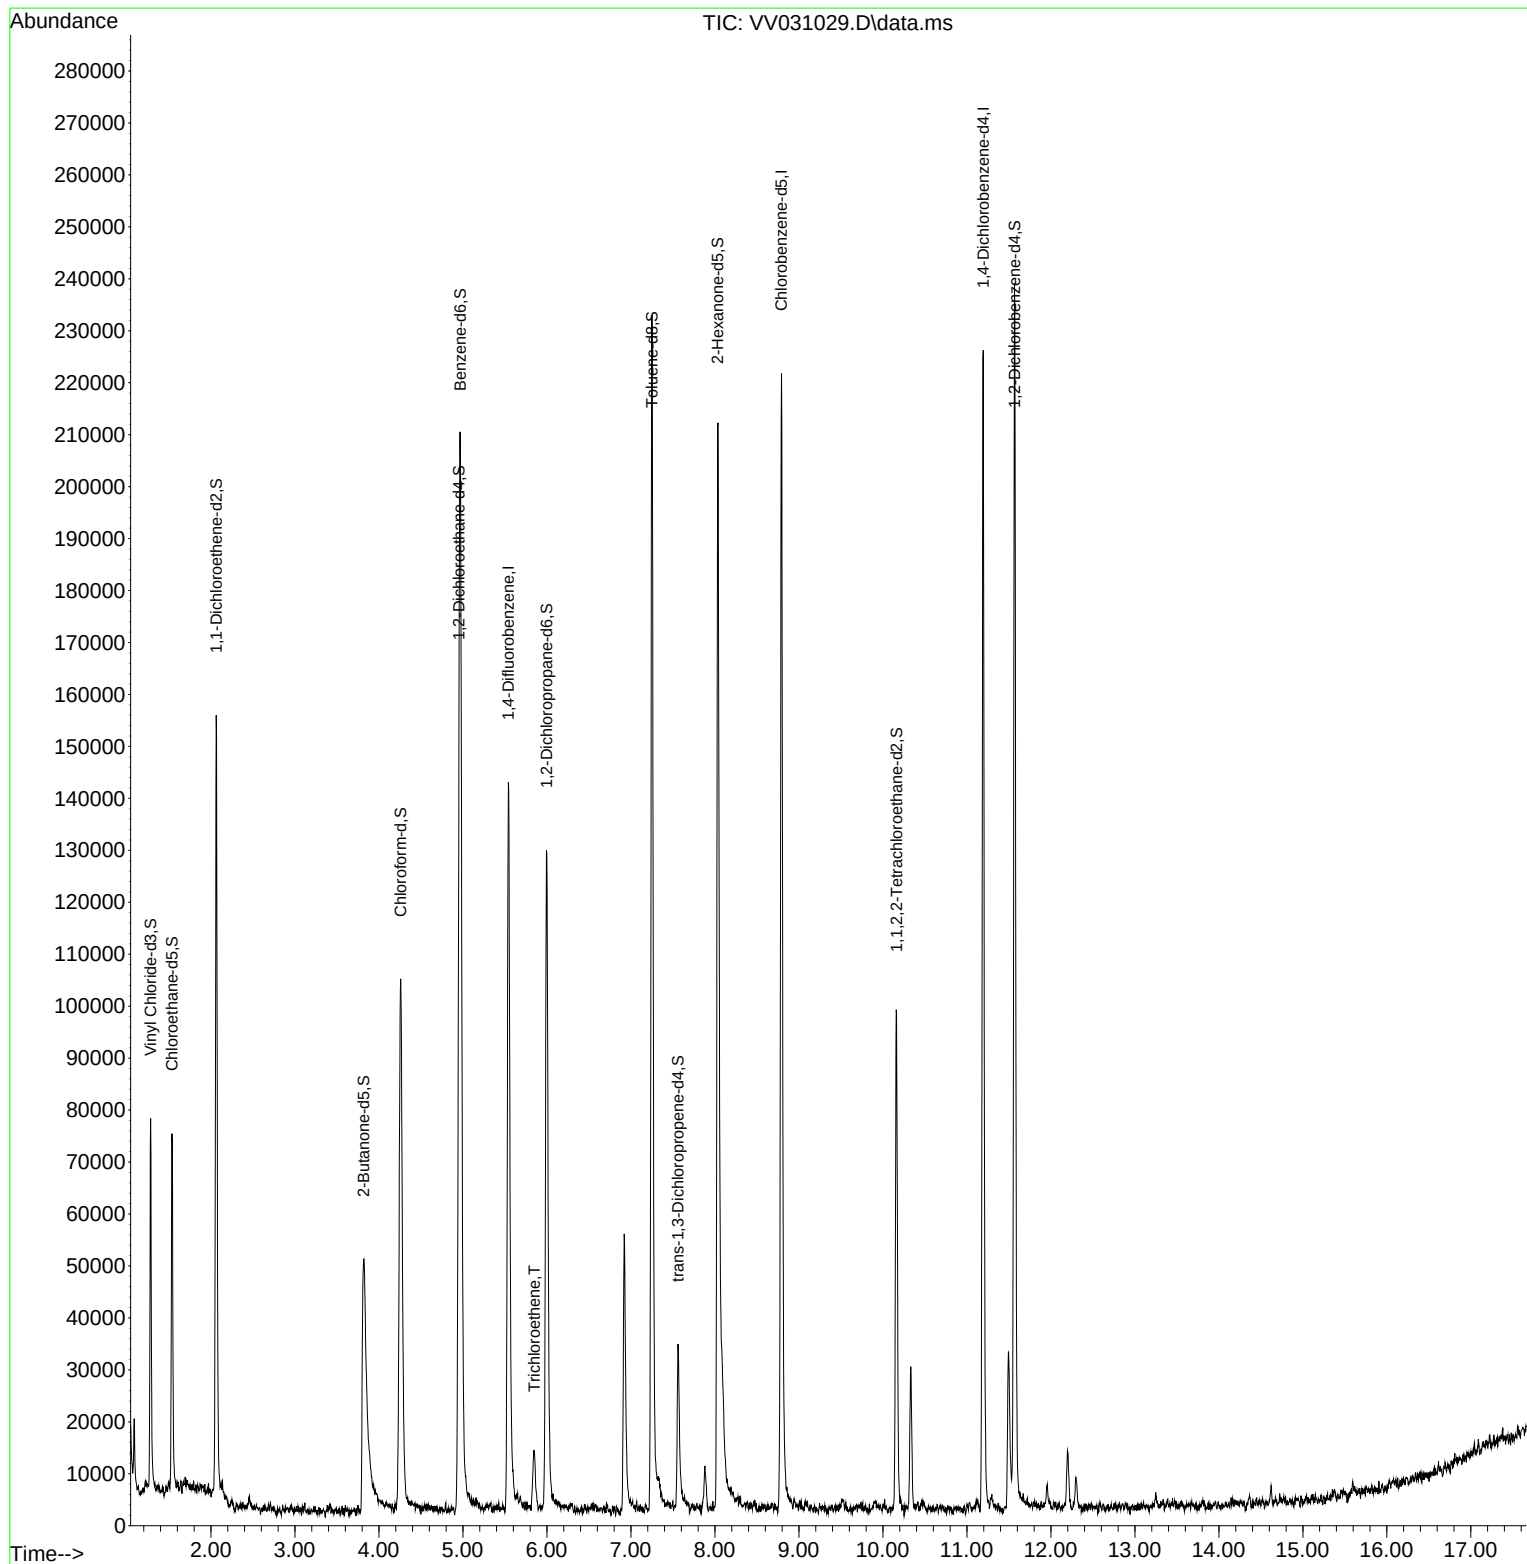

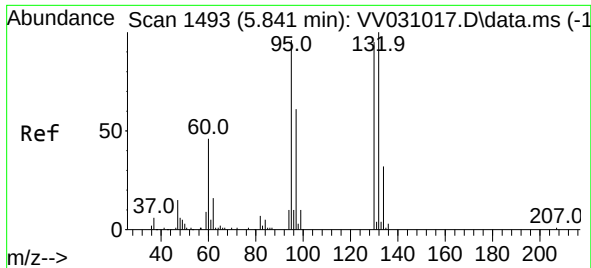

#34
 Trichloroethene
 Concen: 0.437 ug/L
 RT: 5.850 min Scan# 1496
 Delta R.T. 0.010 min
 Lab File: VV031029.D
 Acq: 15 May 2023 16:29

Instrument :
 MSVOA_V
 ClientSampleId :
 CONP3

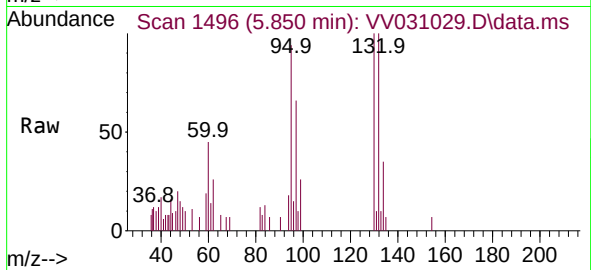

Tgt Ion:	95	Resp:	3591
Ion	Ratio	Lower	Upper
95	100		
97	70.3	46.2	85.8
132	106.5	72.7	135.1
130	106.7	75.7	140.5

