

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051523\
 Data File : VV031030.D
 Acq On : 15 May 2023 16:54
 Operator : SY/MD
 Sample : 02768-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CONP8

Quant Time: May 16 00:16:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue May 16 00:10:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	127911	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	126073	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	63015	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	41807	3.967	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.400%
7) Chloroethane-d5	1.539	69	40311	4.689	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.800%
11) 1,1-Dichloroethene-d2	2.063	65	23042	4.131	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.600%
20) 2-Butanone-d5	3.822	46	94844	50.751	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.500%
24) Chloroform-d	4.259	84	98408	4.699	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.000%
26) 1,2-Dichloroethane-d4	4.953	65	52441	4.925	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.600%
32) Benzene-d6	4.969	84	162798	4.405	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.200%
36) 1,2-Dichloropropane-d6	5.998	67	49654	4.621	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.400%
41) Toluene-d8	7.249	98	139544	3.965	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.400%
43) trans-1,3-Dichloroprop...	7.564	79	16978	4.215	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.200%
46) 2-Hexanone-d5	8.034	63	65288	46.262	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.520%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	37045	4.756	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.200%
66) 1,2-Dichlorobenzene-d4	11.567	152	56142	4.779	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.600%
Target Compounds						
					Qvalue	
34) Trichloroethene	5.847	95	3635	0.430	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051523\
Data File : VV031030.D
Acq On : 15 May 2023 16:54
Operator : SY/MD
Sample : 02768-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONP8


Quant Time: May 16 00:16:37 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue May 16 00:10:06 2023
Response via : Initial Calibration

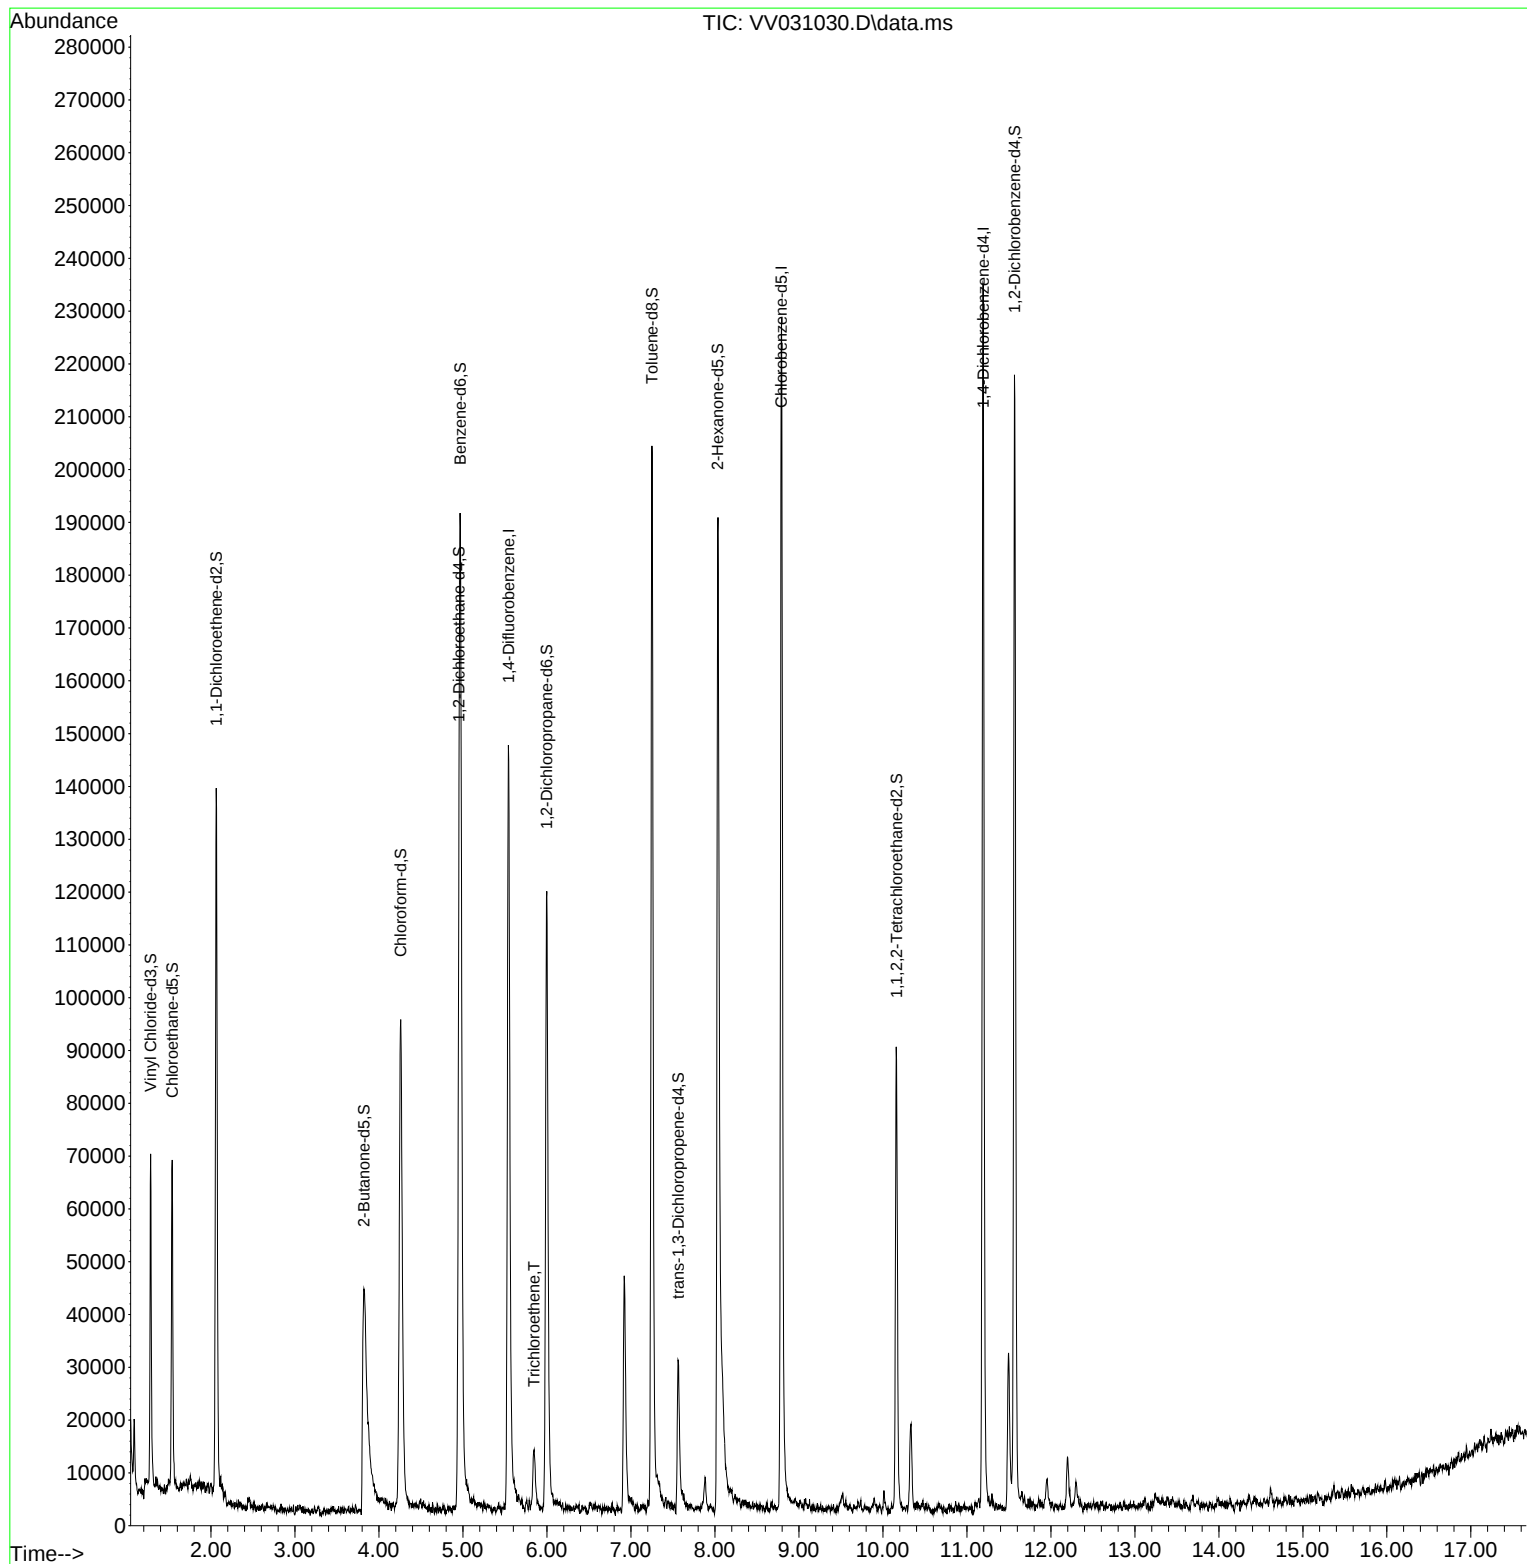

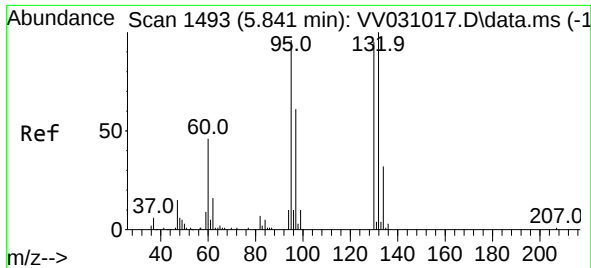

#34
 Trichloroethene
 Concen: 0.430 ug/L
 RT: 5.847 min Scan# 1493
 Delta R.T. 0.006 min
 Lab File: VV031030.D
 Acq: 15 May 2023 16:54

Instrument :
 MSVOA_V
 ClientSampleId :
 CONP8

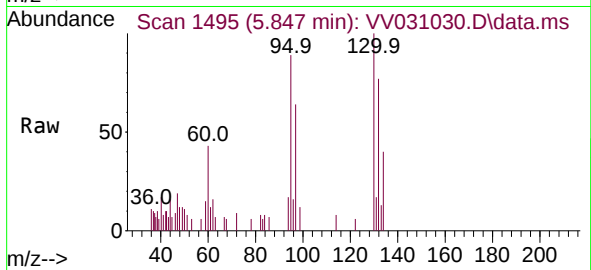

Tgt Ion: 95	Resp: 3635
Ion Ratio	Lower Upper
95 100	
97 72.4	46.2 85.8
132 86.8	72.7 135.1
130 112.4	75.7 140.5

