

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051523\
 Data File : VV031032.D
 Acq On : 15 May 2023 17:43
 Operator : SY/MD
 Sample : VV0515WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK337

Quant Time: May 16 00:42:49 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue May 16 00:40:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	125974	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	123081	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	61450	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	41717	4.019	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	80.400%	
7) Chloroethane-d5	1.535	69	39911	4.714	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	94.200%	
11) 1,1-Dichloroethene-d2	2.063	65	22833	4.157	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	83.200%	
20) 2-Butanone-d5	3.828	46	98383	53.454	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	106.900%	
24) Chloroform-d	4.259	84	97367	4.720	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.400%	
26) 1,2-Dichloroethane-d4	4.953	65	54572	5.204	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	104.000%	
32) Benzene-d6	4.969	84	168413	4.668	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.400%	
36) 1,2-Dichloropropane-d6	5.998	67	50019	4.768	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	95.400%	
41) Toluene-d8	7.252	98	141315	4.113	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	82.200%	
43) trans-1,3-Dichloroprop...	7.564	79	18295	4.652	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	93.000%	
46) 2-Hexanone-d5	8.037	63	69359	50.341	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	100.680%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84	38654	5.083	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	101.600%	
66) 1,2-Dichlorobenzene-d4	11.570	152	56437	4.927	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	98.600%	
Target Compounds						Qvalue
34) Trichloroethene	5.844	95	3152	0.382	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051523\
Data File : VV031032.D
Acq On : 15 May 2023 17:43
Operator : SY/MD
Sample : VV0515WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK337


Quant Time: May 16 00:42:49 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue May 16 00:40:05 2023
Response via : Initial Calibration

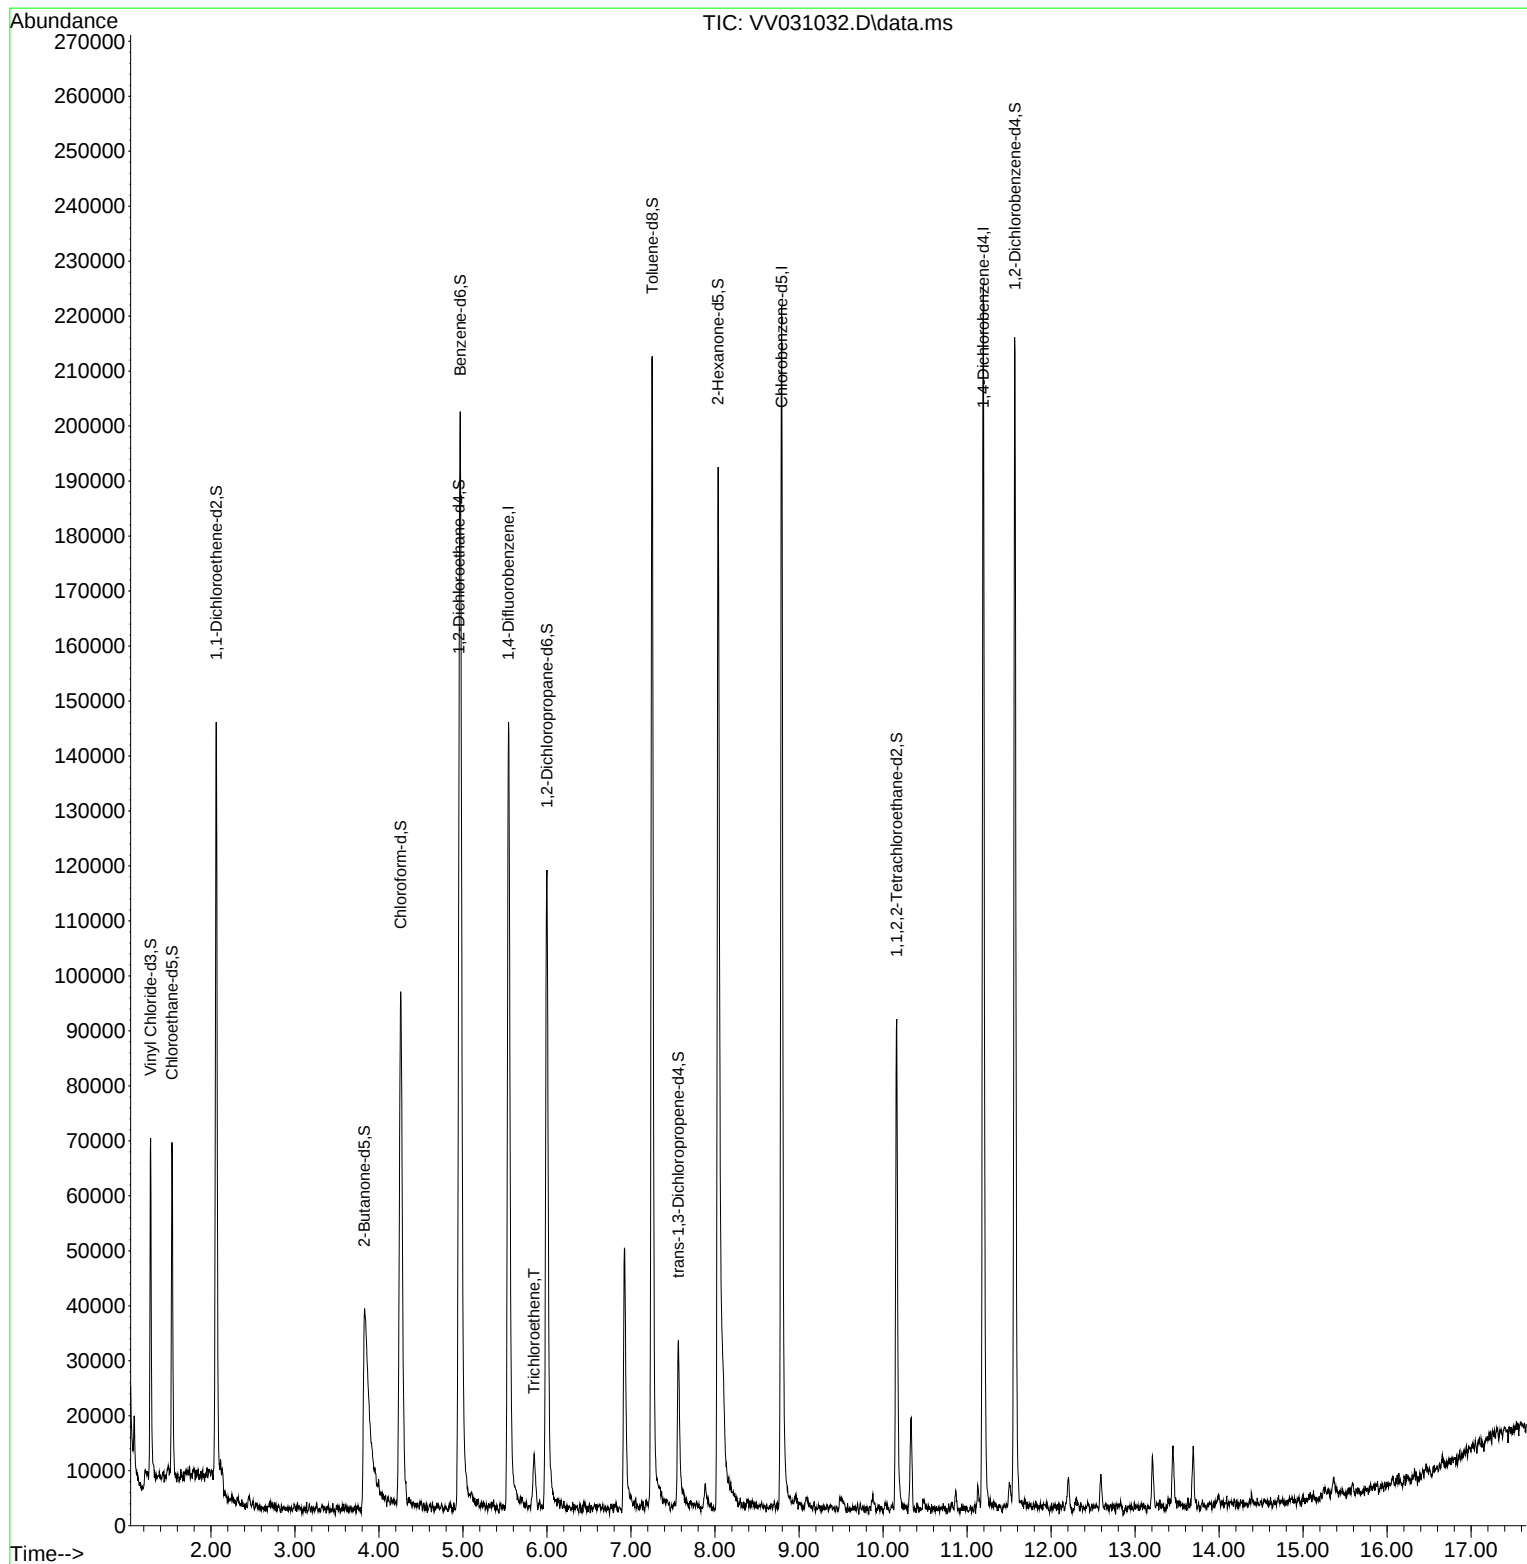

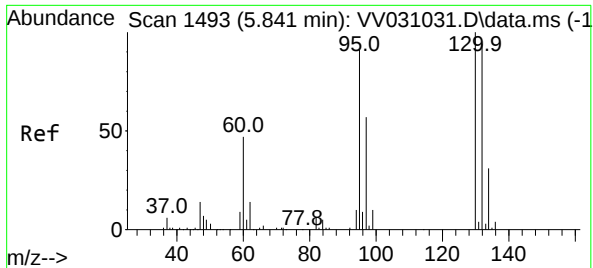

#34
 Trichloroethene
 Concen: 0.382 ug/L
 RT: 5.844 min Scan# 1494
 Delta R.T. 0.003 min
 Lab File: VV031032.D
 Acq: 15 May 2023 17:43

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK337

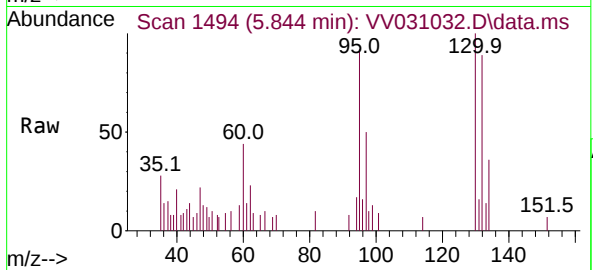

Tgt Ion: 95 Resp: 3152

Ion	Ratio	Lower	Upper
95	100		
97	54.7	46.2	85.8
132	96.3	72.7	135.1
130	108.7	75.7	140.5

