

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051523\
 Data File : VV031034.D
 Acq On : 15 May 2023 18:32
 Operator : SY/MD
 Sample : 02768-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CONN9

Quant Time: May 16 00:45:48 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue May 16 00:40:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	124510	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	121201	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	60202	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	40621	3.960	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.200%
7) Chloroethane-d5	1.536	69	39094	4.672	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.400%
11) 1,1-Dichloroethene-d2	2.063	65	22319	4.111	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.200%
20) 2-Butanone-d5	3.822	46	99980	54.961	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.920%
24) Chloroform-d	4.259	84	95391	4.679	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.600%
26) 1,2-Dichloroethane-d4	4.954	65	52294	5.045	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.000%
32) Benzene-d6	4.970	84	162236	4.567	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.400%
36) 1,2-Dichloropropane-d6	5.995	67	48160	4.662	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.200%
41) Toluene-d8	7.252	98	135688	4.011	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.200%
43) trans-1,3-Dichloroprop...	7.561	79	17320	4.473	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.400%
46) 2-Hexanone-d5	8.037	63	66055	48.687	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.380%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	39494	5.274	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.400%
66) 1,2-Dichlorobenzene-d4	11.571	152	55461	4.942	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.800%
Target Compounds						
					Qvalue	
34) Trichloroethene	5.847	95	2461	0.303	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051523\
Data File : VV031034.D
Acq On : 15 May 2023 18:32
Operator : SY/MD
Sample : 02768-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONN9


Quant Time: May 16 00:45:48 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue May 16 00:40:05 2023
Response via : Initial Calibration

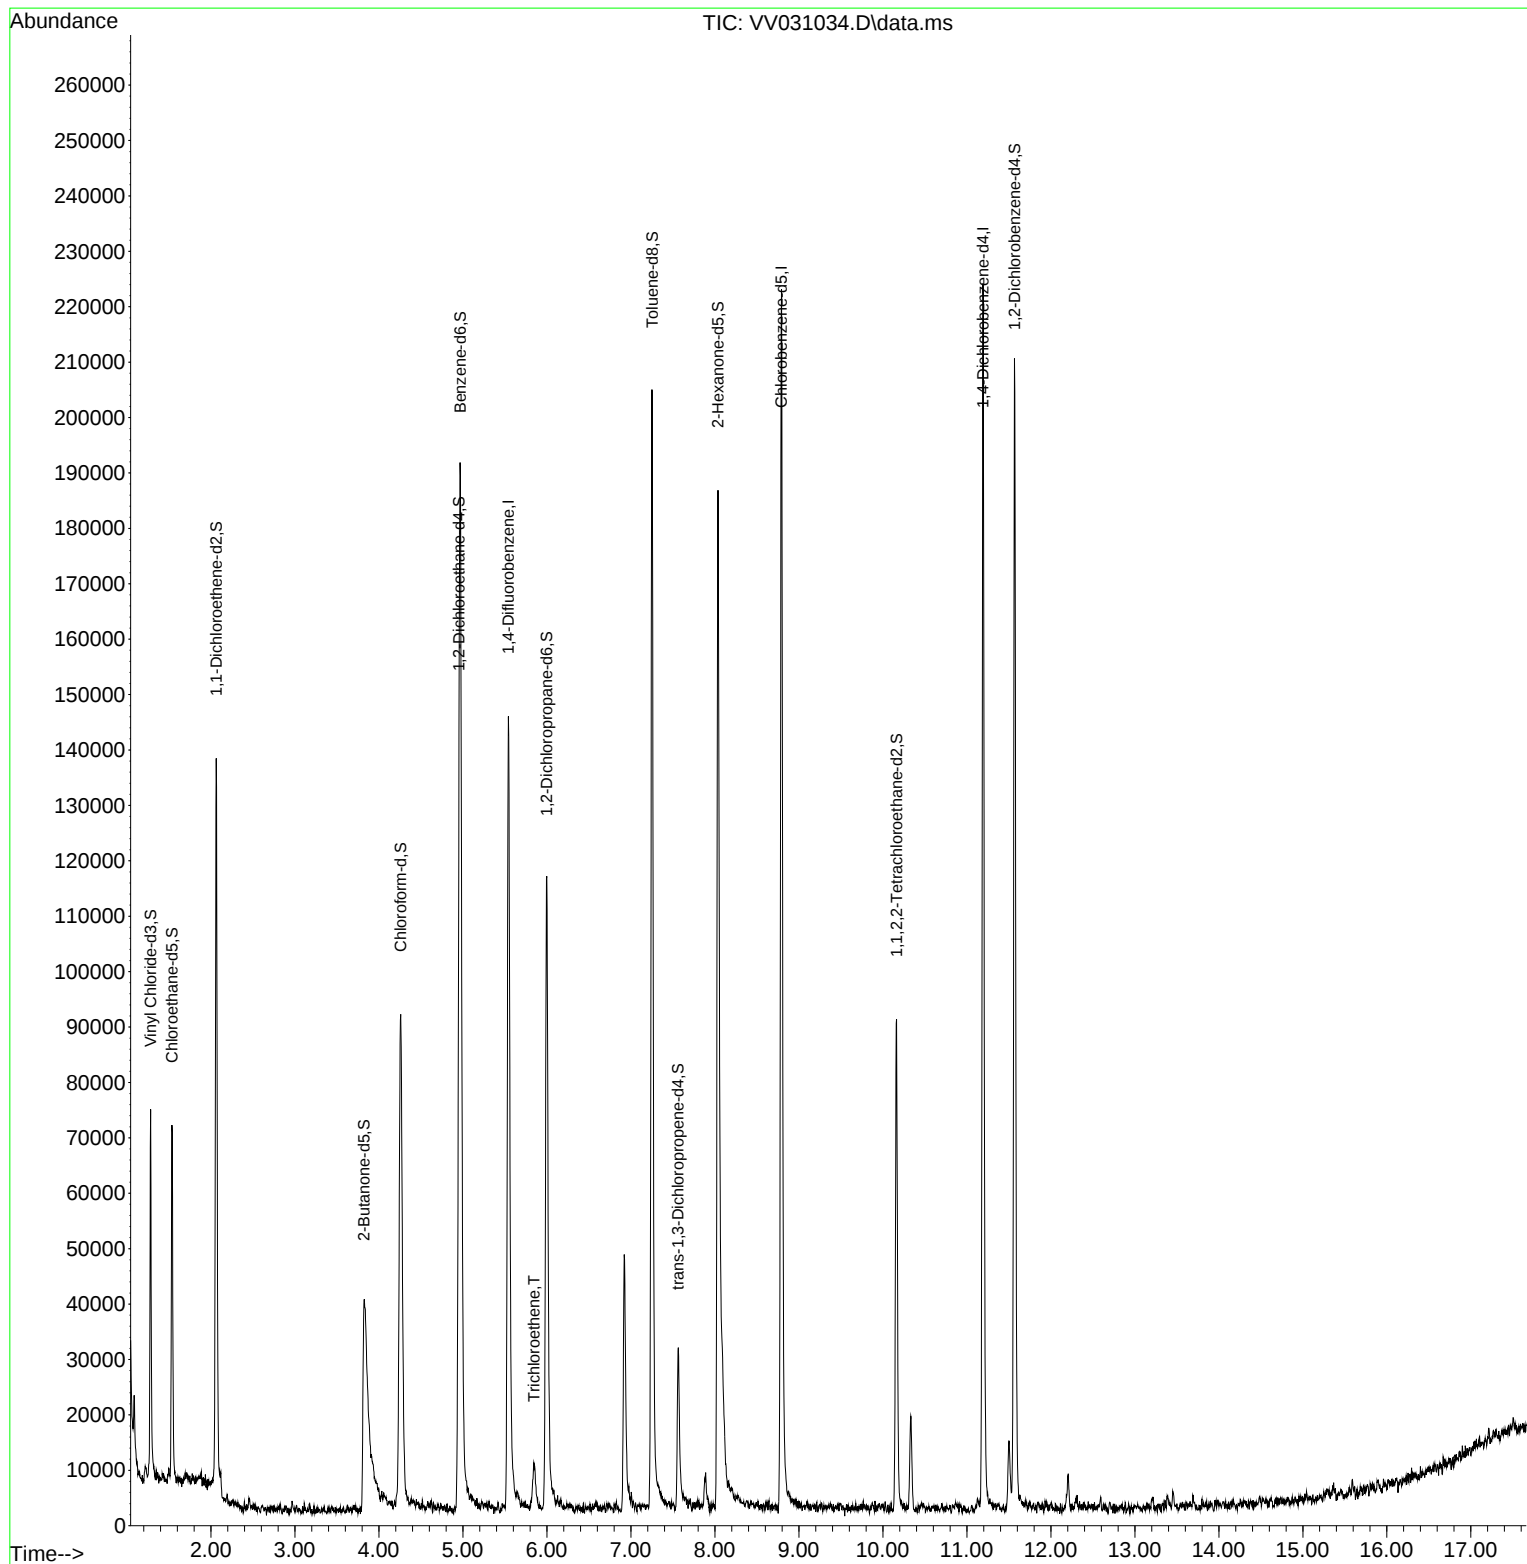

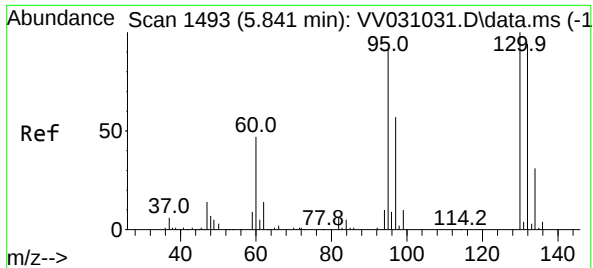

#34
 Trichloroethene
 Concen: 0.303 ug/L
 RT: 5.847 min Scan# 1495
 Delta R.T. 0.007 min
 Lab File: VV031034.D
 Acq: 15 May 2023 18:32

Instrument :
 MSVOA_V
 ClientSampleId :
 CONN9

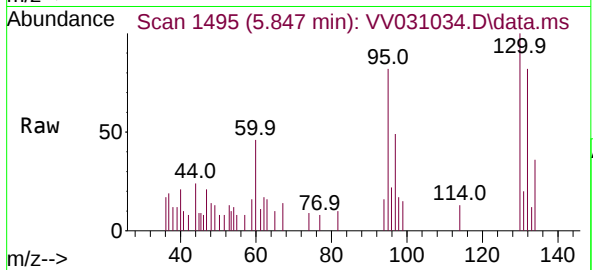

Tgt Ion: 95 Resp: 2461

Ion	Ratio	Lower	Upper
95	100		
97	59.2	46.2	85.8
132	99.4	72.7	135.1
130	121.4	75.7	140.5

