

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051523\
 Data File : VV031035.D
 Acq On : 15 May 2023 18:57
 Operator : SY/MD
 Sample : 02768-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CONP2

Quant Time: May 16 00:46:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue May 16 00:40:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	125003	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	125010	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	63232	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	41497	4.029	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.600%
7) Chloroethane-d5	1.539	69	42449	5.053	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.000%
11) 1,1-Dichloroethene-d2	2.066	65	23585	4.327	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	86.600%
20) 2-Butanone-d5	3.818	46	102593	56.175	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	112.340%
24) Chloroform-d	4.259	84	104704	5.116	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.400%
26) 1,2-Dichloroethane-d4	4.953	65	55177	5.303	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.000%
32) Benzene-d6	4.969	84	175640	4.793	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.800%
36) 1,2-Dichloropropane-d6	5.998	67	51679	4.850	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.000%
41) Toluene-d8	7.249	98	148787	4.264	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.200%
43) trans-1,3-Dichloroprop...	7.564	79	18856	4.721	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.400%
46) 2-Hexanone-d5	8.034	63	70231	50.188	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.380%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	39785	5.151	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.000%
66) 1,2-Dichlorobenzene-d4	11.570	152	60863	5.164	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.200%
Target Compounds						Qvalue
34) Trichloroethene	5.850	95	2099	0.250	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051523\
Data File : VV031035.D
Acq On : 15 May 2023 18:57
Operator : SY/MD
Sample : 02768-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONP2


Quant Time: May 16 00:46:01 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue May 16 00:40:05 2023
Response via : Initial Calibration

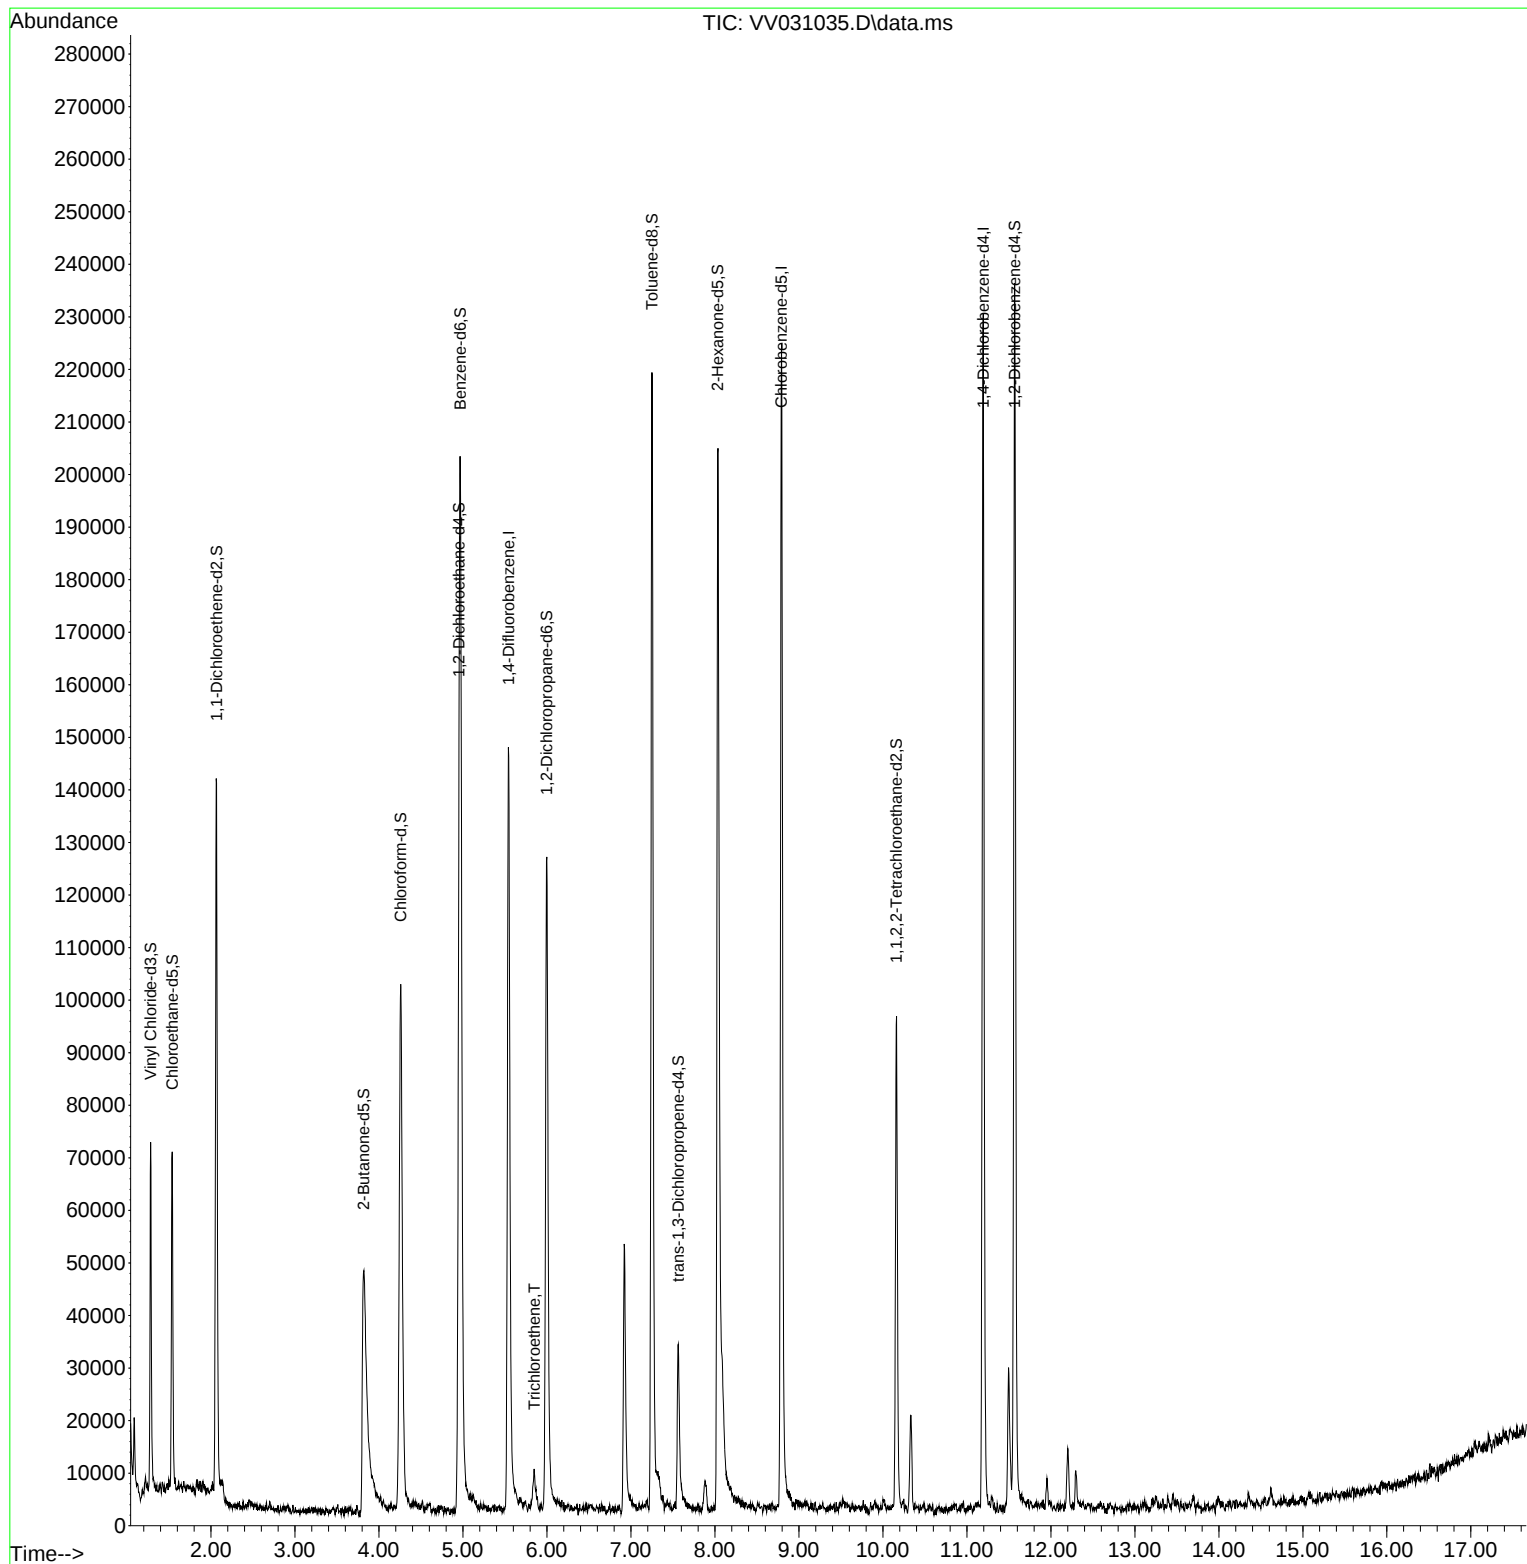

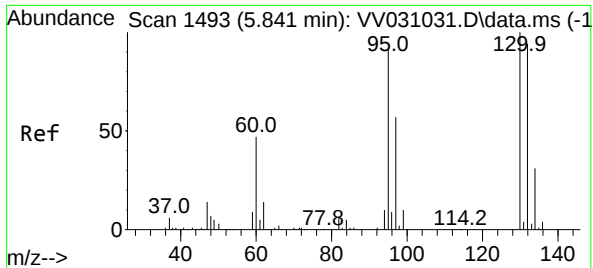

#34
 Trichloroethene
 Concen: 0.250 ug/L
 RT: 5.850 min Scan# 1496
 Delta R.T. 0.010 min
 Lab File: VV031035.D
 Acq: 15 May 2023 18:57

Instrument :
 MSVOA_V
 ClientSampleId :
 CONP2

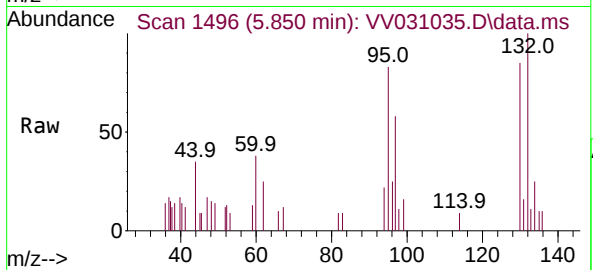

Tgt Ion: 95 Resp: 2099

Ion	Ratio	Lower	Upper
95	100		
97	69.5	46.2	85.8
132	120.7	72.7	135.1
130	102.9	75.7	140.5

