

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051523\
 Data File : VV031032.D
 Acq On : 15 May 2023 17:43
 Operator : SY/MD
 Sample : VV0515WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK337

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV031032.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	10	14	24	rVB2	10799	11918	2.31%	0.284%
2	1.281	67	75	86	rBV	62038	71721	13.90%	1.706%
3	1.535	147	154	167	rVB	60928	73296	14.21%	1.744%
4	2.063	306	318	331	rBV	137830	204846	39.70%	4.873%
5	3.828	855	867	892	rBV2	37167	155453	30.13%	3.698%
6	4.259	986	1001	1019	rBV	93339	240400	46.59%	5.719%
7	4.966	1203	1221	1248	rBV3	199775	515971	100.00%	12.275%
8	5.542	1388	1400	1422	rBV	142990	307506	59.60%	7.315%
9	5.847	1482	1495	1509	rVB	10169	23272	4.51%	0.554%
10	5.998	1529	1542	1562	rBV	116090	251663	48.77%	5.987%
11	6.921	1819	1829	1843	rBV2	48090	95327	18.48%	2.268%
12	7.252	1917	1932	1950	rBV	209184	382810	74.19%	9.107%
13	7.564	2019	2029	2043	rBV	30150	56811	11.01%	1.352%
14	7.882	2117	2128	2135	rBV4	4539	8004	1.55%	0.190%
15	8.037	2165	2176	2206	rBV	189558	447149	86.66%	10.638%
16	8.792	2400	2411	2432	rBV	218431	378021	73.26%	8.993%
17	10.162	2826	2837	2857	rBV	89327	150288	29.13%	3.575%
18	10.336	2878	2891	2900	rBV	17572	30450	5.90%	0.724%
19	10.866	3049	3056	3064	rVB	3763	5411	1.05%	0.129%
20	11.127	3129	3137	3142	rBV10	5203	7181	1.39%	0.171%
21	11.194	3147	3158	3180	rVV	222964	368953	71.51%	8.777%
22	11.567	3263	3274	3292	rVB	211988	345641	66.99%	8.223%
23	12.207	3457	3473	3482	rBV4	6123	12197	2.36%	0.290%
24	12.593	3585	3593	3602	rBV10	6569	10548	2.04%	0.251%
25	13.207	3775	3784	3796	rBV8	9714	15920	3.09%	0.379%
26	13.451	3852	3860	3869	rBV	10511	16422	3.18%	0.391%
27	13.693	3926	3935	3943	rBV7	10917	16332	3.17%	0.389%




Sum of corrected areas: 4203511

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051523\
Data File : VV031032.D
Acq On : 15 May 2023 17:43
Operator : SY/MD
Sample : VV0515WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK337

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

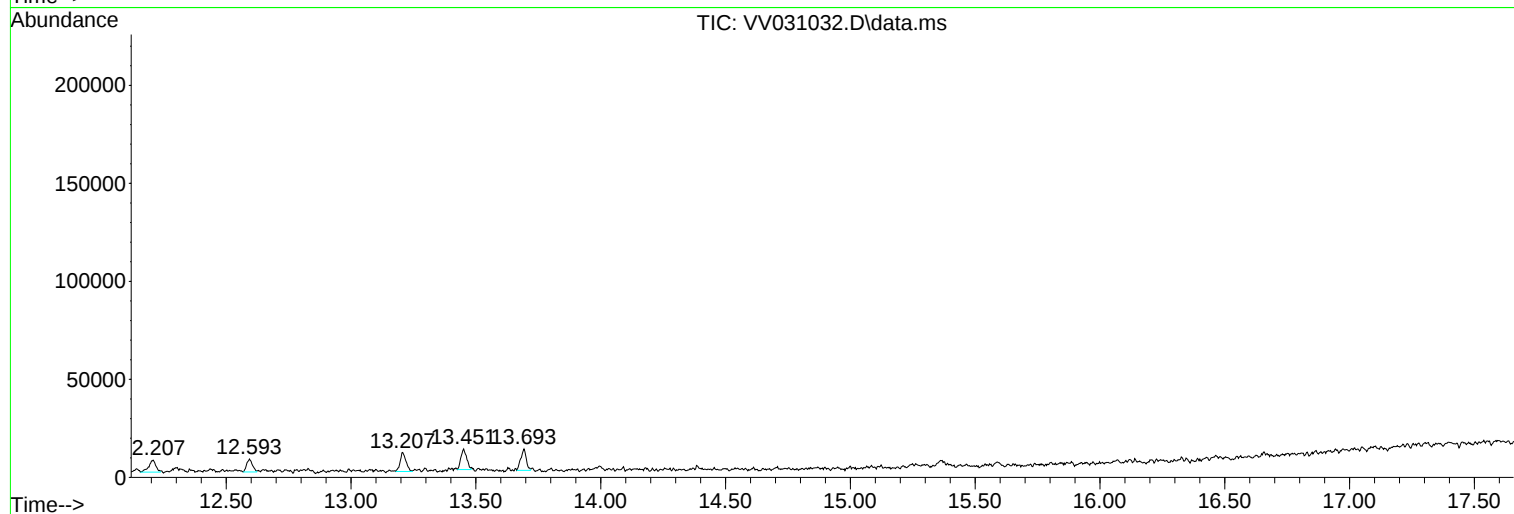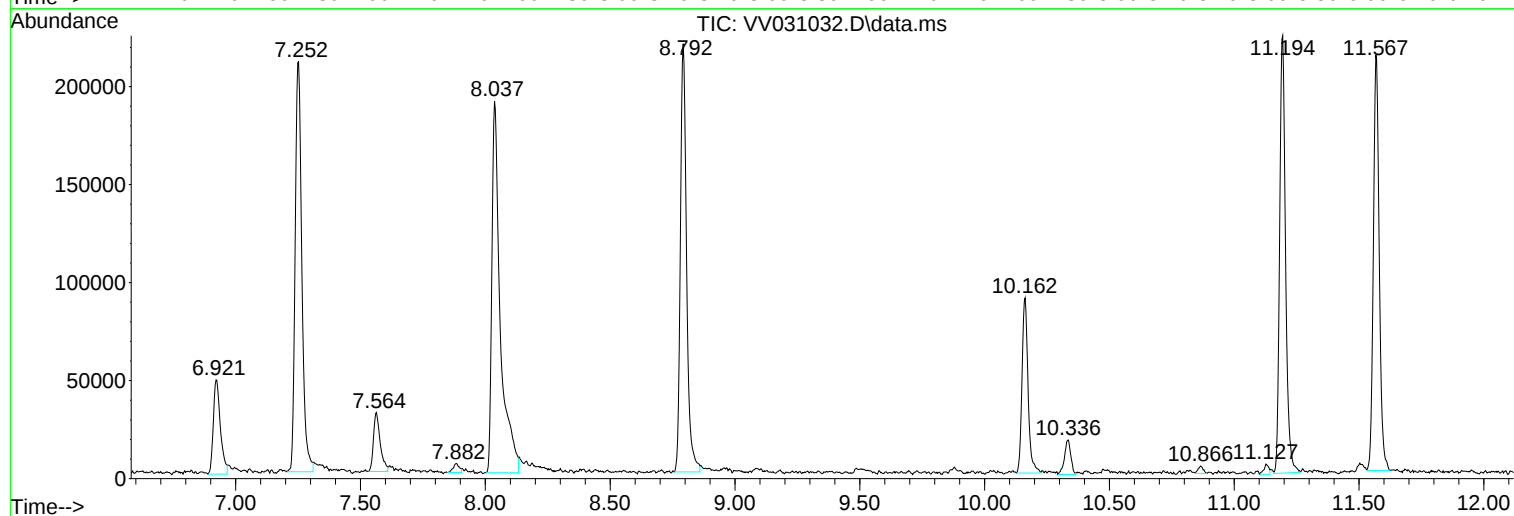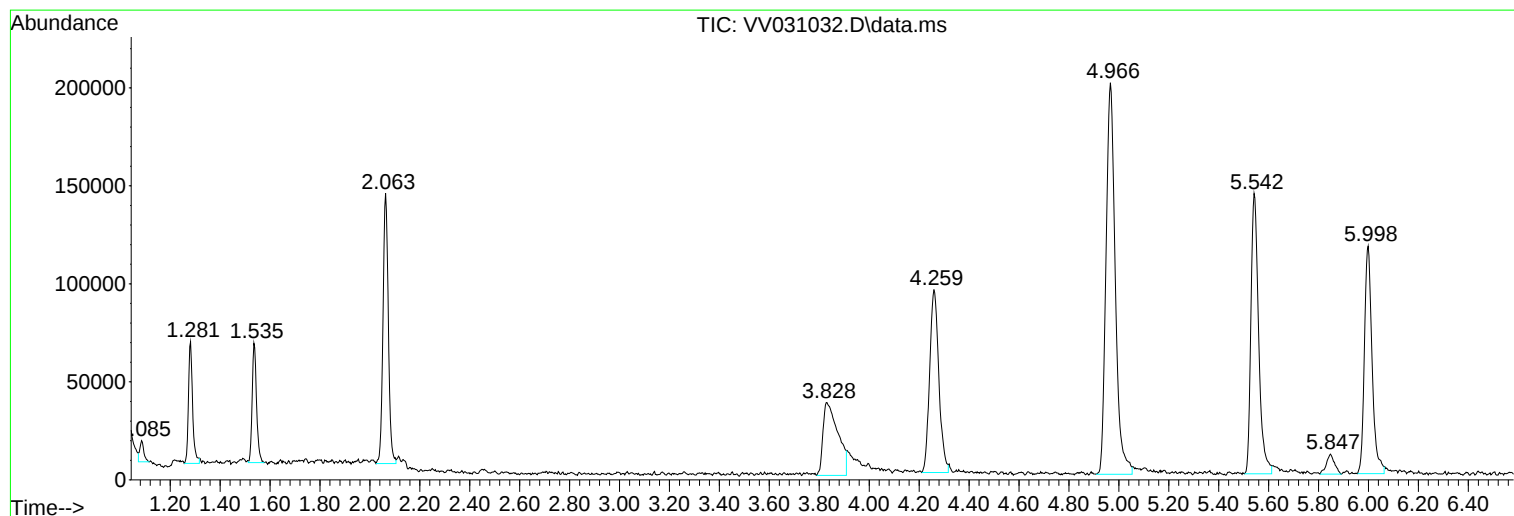

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051523\
Data File : VV031032.D
Acq On : 15 May 2023 17:43
Operator : SY/MD
Sample : VV0515WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK337

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051523\
Data File : VV031032.D
Acq On : 15 May 2023 17:43
Operator : SY/MD
Sample : VV0515WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK337

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------