

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051523\
 Data File : VV031033.D
 Acq On : 15 May 2023 18:08
 Operator : SY/MD
 Sample : 02768-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CONN2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031033.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	84	rBV	61950	65035	12.66%	1.527%
2	1.536	145	154	168	rVB	67491	83733	16.30%	1.966%
3	2.063	308	318	332	rBV	137536	199311	38.79%	4.679%
4	3.822	855	865	900	rBV2	45824	189211	36.82%	4.442%
5	4.252	985	999	1024	rBV2	94742	250624	48.78%	5.884%
6	4.966	1204	1221	1244	rBV2	194490	513835	100.00%	12.064%
7	5.542	1388	1400	1422	rBV	145737	305378	59.43%	7.170%
8	5.854	1480	1497	1503	rBV	8435	18323	3.57%	0.430%
9	5.995	1526	1541	1561	rBV2	120823	264826	51.54%	6.218%
10	6.921	1819	1829	1847	rBV2	46633	94760	18.44%	2.225%
11	7.249	1917	1931	1953	rBV	214661	392101	76.31%	9.206%
12	7.564	2020	2029	2042	rBV2	29066	55381	10.78%	1.300%
13	7.879	2119	2127	2140	rBV4	10180	18845	3.67%	0.442%
14	8.037	2163	2176	2215	rBV	201517	476542	92.74%	11.188%
15	8.792	2399	2411	2433	rBV	215351	377315	73.43%	8.859%
16	10.162	2823	2837	2853	rBV	93069	155792	30.32%	3.658%
17	10.336	2882	2891	2900	rVB	28963	48092	9.36%	1.129%
18	11.191	3145	3157	3176	rVV	220782	360156	70.09%	8.456%
19	11.500	3239	3253	3262	rBV8	10019	19850	3.86%	0.466%
20	11.567	3262	3274	3292	rVB	218305	357237	69.52%	8.387%
21	12.207	3462	3473	3482	rBV	9113	12987	2.53%	0.305%




Sum of corrected areas: 4259334

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051523\
Data File : VV031033.D
Acq On : 15 May 2023 18:08
Operator : SY/MD
Sample : 02768-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONN2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

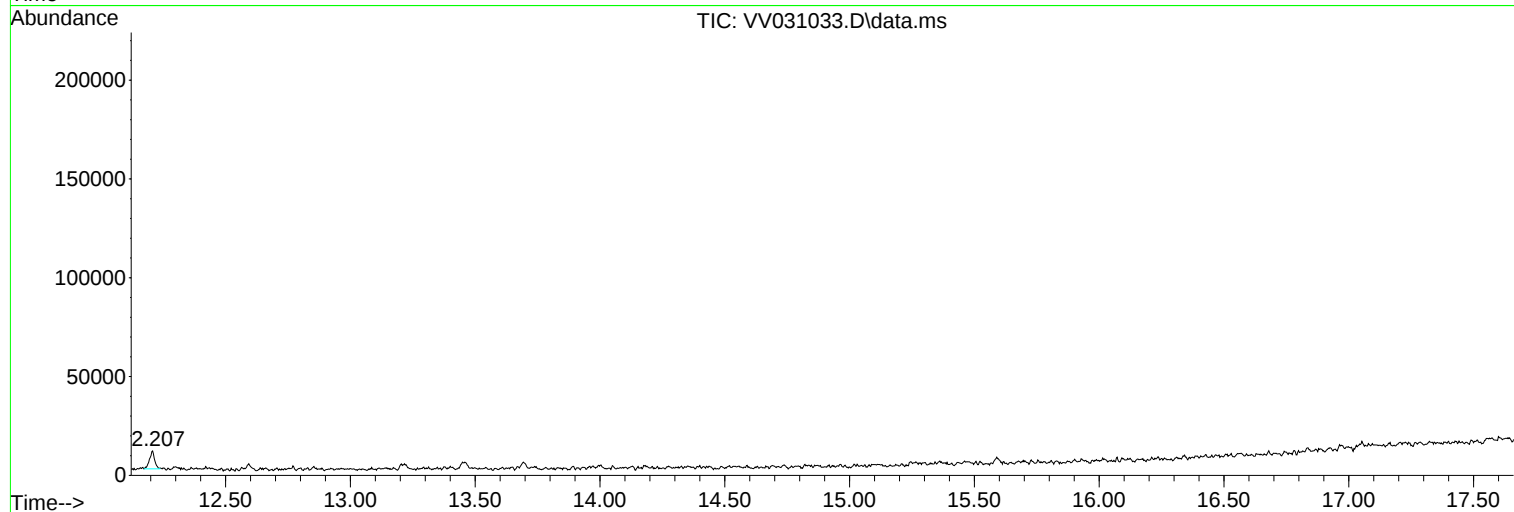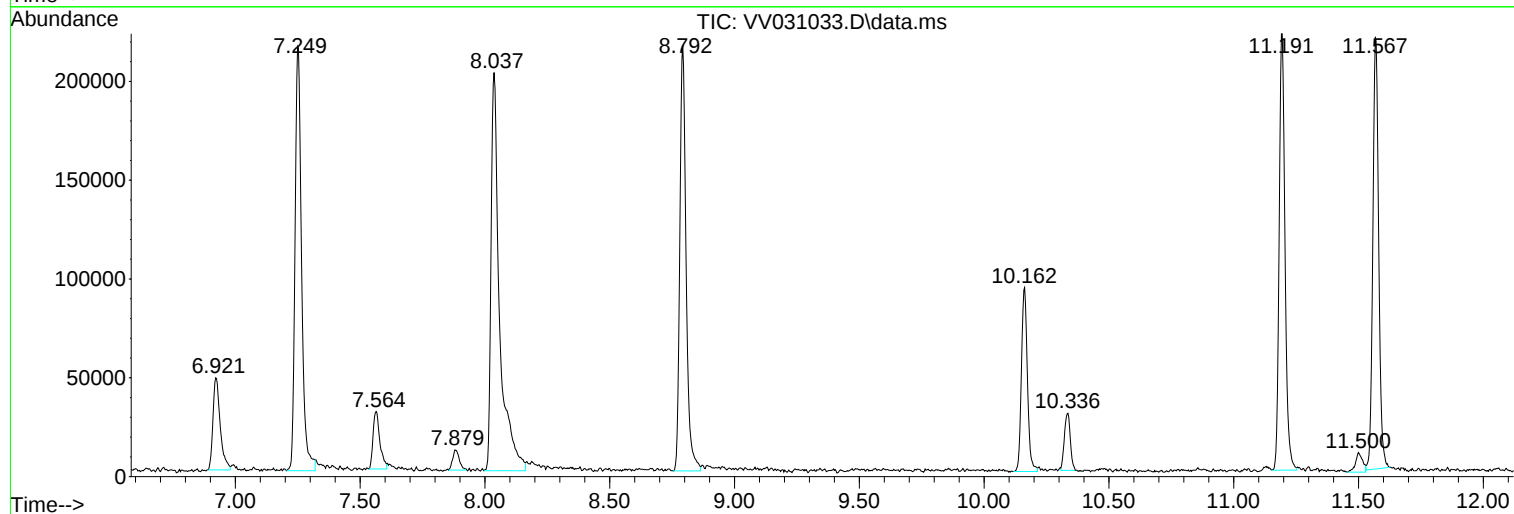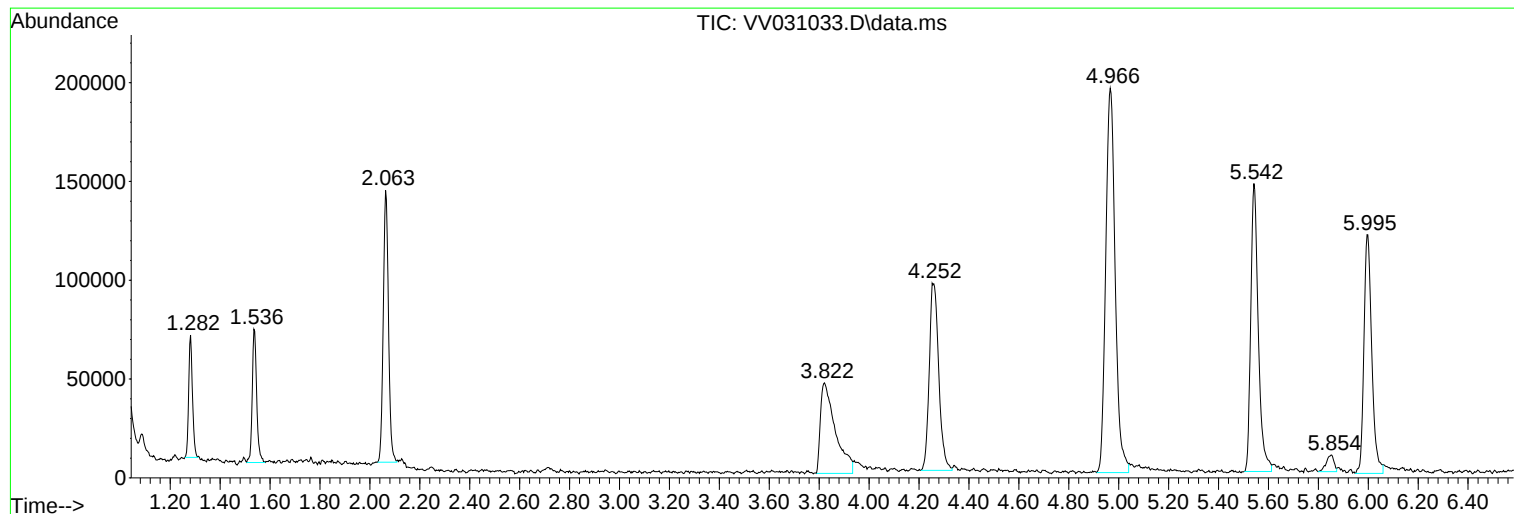

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051523\
Data File : VV031033.D
Acq On : 15 May 2023 18:08
Operator : SY/MD
Sample : 02768-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONN2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051523\
Data File : VV031033.D
Acq On : 15 May 2023 18:08
Operator : SY/MD
Sample : 02768-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONN2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------