

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051523\
 Data File : VV031034.D
 Acq On : 15 May 2023 18:32
 Operator : SY/MD
 Sample : 02768-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CONN9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV031034.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.086	11	14	23	rVB2	12240	13267	2.71%	0.328%
2	1.282	66	75	90	rVB	66331	71768	14.68%	1.773%
3	1.536	147	154	170	rVB	64571	79276	16.21%	1.958%
4	2.063	307	318	330	rBV	129807	186640	38.17%	4.611%
5	3.825	855	866	891	rBV2	38329	151725	31.03%	3.748%
6	4.259	982	1001	1025	rBV2	88932	238350	48.74%	5.888%
7	4.966	1204	1221	1244	rBV2	189050	488988	100.00%	12.080%
8	5.542	1388	1400	1427	rBV	142926	307667	62.92%	7.600%
9	5.844	1485	1494	1496	rBV9	7249	9148	1.87%	0.226%
10	5.998	1527	1542	1562	rBV2	114036	244727	50.05%	6.046%
11	6.921	1816	1829	1844	rBV2	46501	92522	18.92%	2.286%
12	7.249	1919	1931	1952	rBV	201958	369701	75.61%	9.133%
13	7.564	2019	2029	2045	rBV2	28819	56025	11.46%	1.384%
14	7.889	2121	2130	2136	rBV4	5971	9394	1.92%	0.232%
15	8.037	2165	2176	2211	rBV	183888	440348	90.05%	10.878%
16	8.793	2399	2411	2433	rBV	220920	388719	79.49%	9.603%
17	10.162	2825	2837	2852	rBV	88603	146846	30.03%	3.628%
18	10.333	2880	2890	2900	rVB2	16816	29113	5.95%	0.719%
19	11.191	3145	3157	3173	rBV	220847	353298	72.25%	8.728%
20	11.500	3244	3253	3263	rBV4	12319	23873	4.88%	0.590%
21	11.567	3263	3274	3290	rVB	206043	337651	69.05%	8.341%
22	12.207	3467	3473	3481	rVB6	6584	9022	1.85%	0.223%




Sum of corrected areas: 4048068

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051523\
Data File : VV031034.D
Acq On : 15 May 2023 18:32
Operator : SY/MD
Sample : 02768-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONN9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

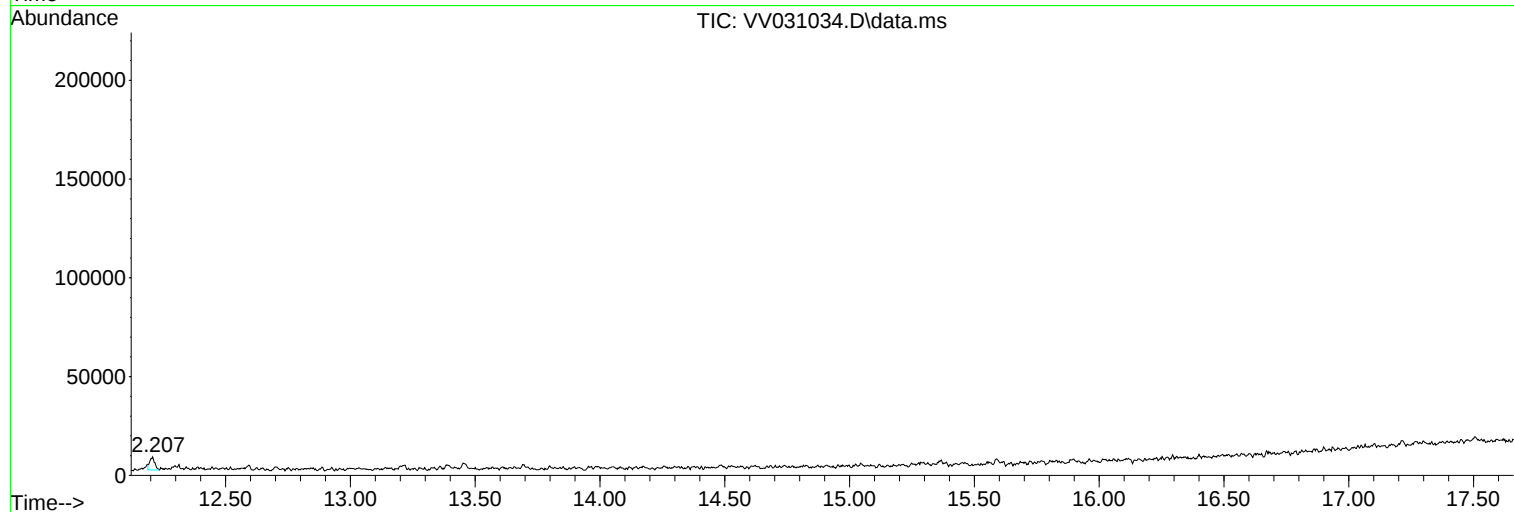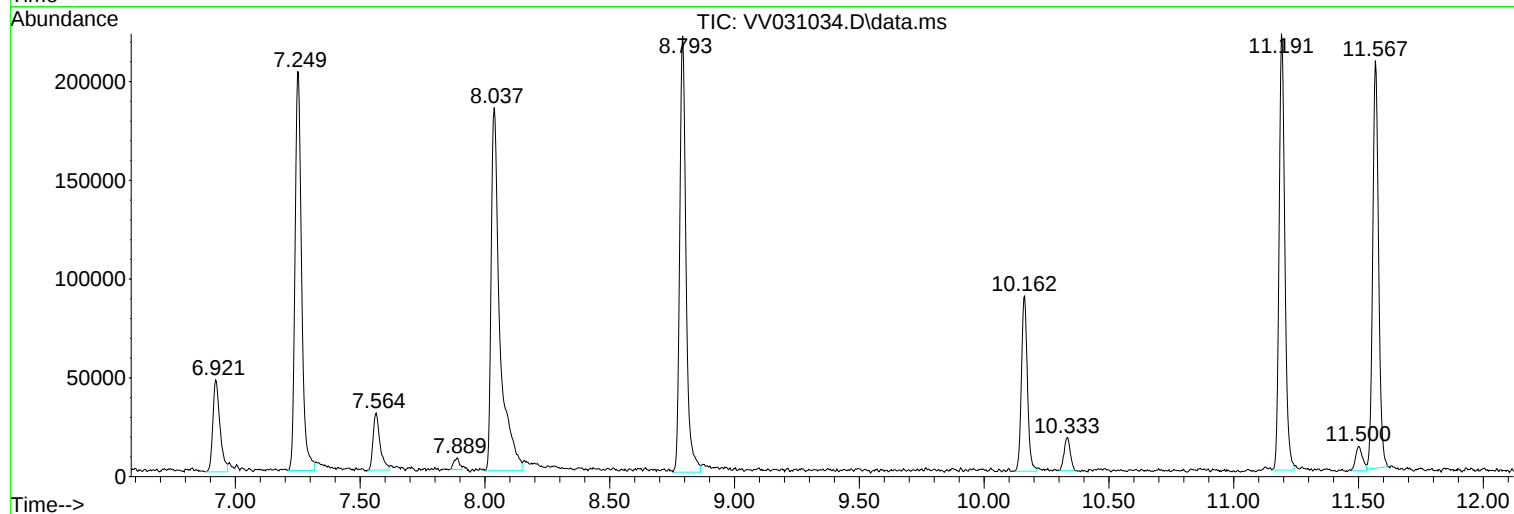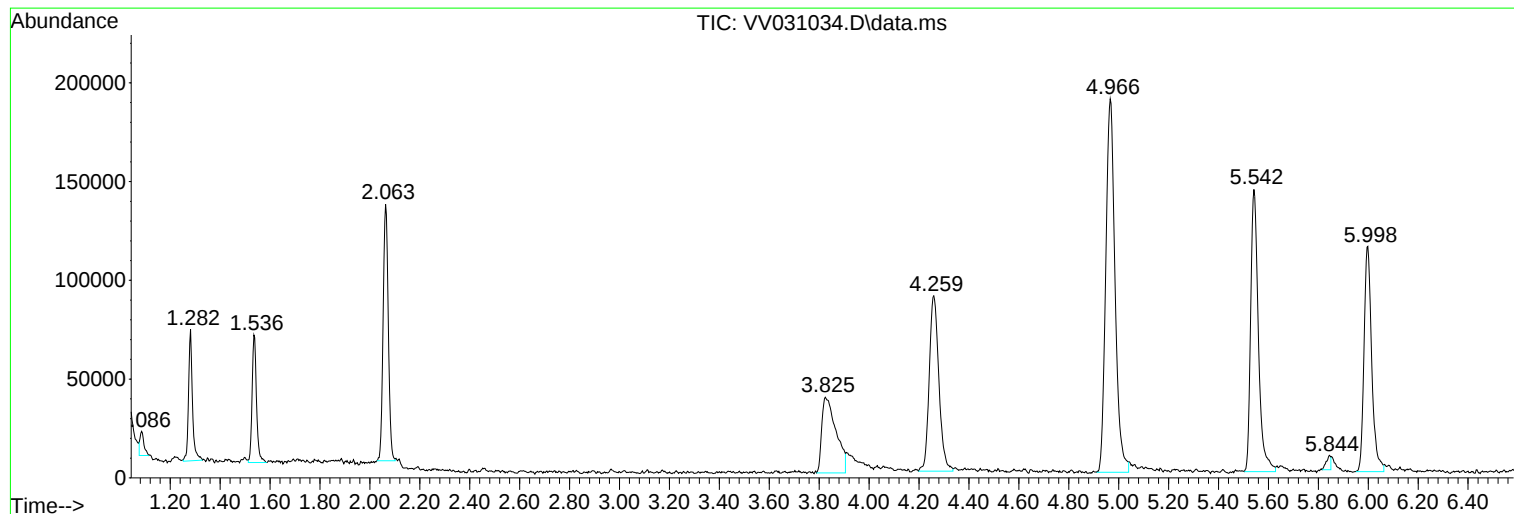

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051523\
Data File : VV031034.D
Acq On : 15 May 2023 18:32
Operator : SY/MD
Sample : 02768-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONN9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051523\
Data File : VV031034.D
Acq On : 15 May 2023 18:32
Operator : SY/MD
Sample : 02768-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONN9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc