


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051523\
 Data File : VV031016.D
 Acq On : 15 May 2023 08:54
 Operator : SY/MD
 Sample : BFB261
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB261

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed May 17 01:41:23 2023

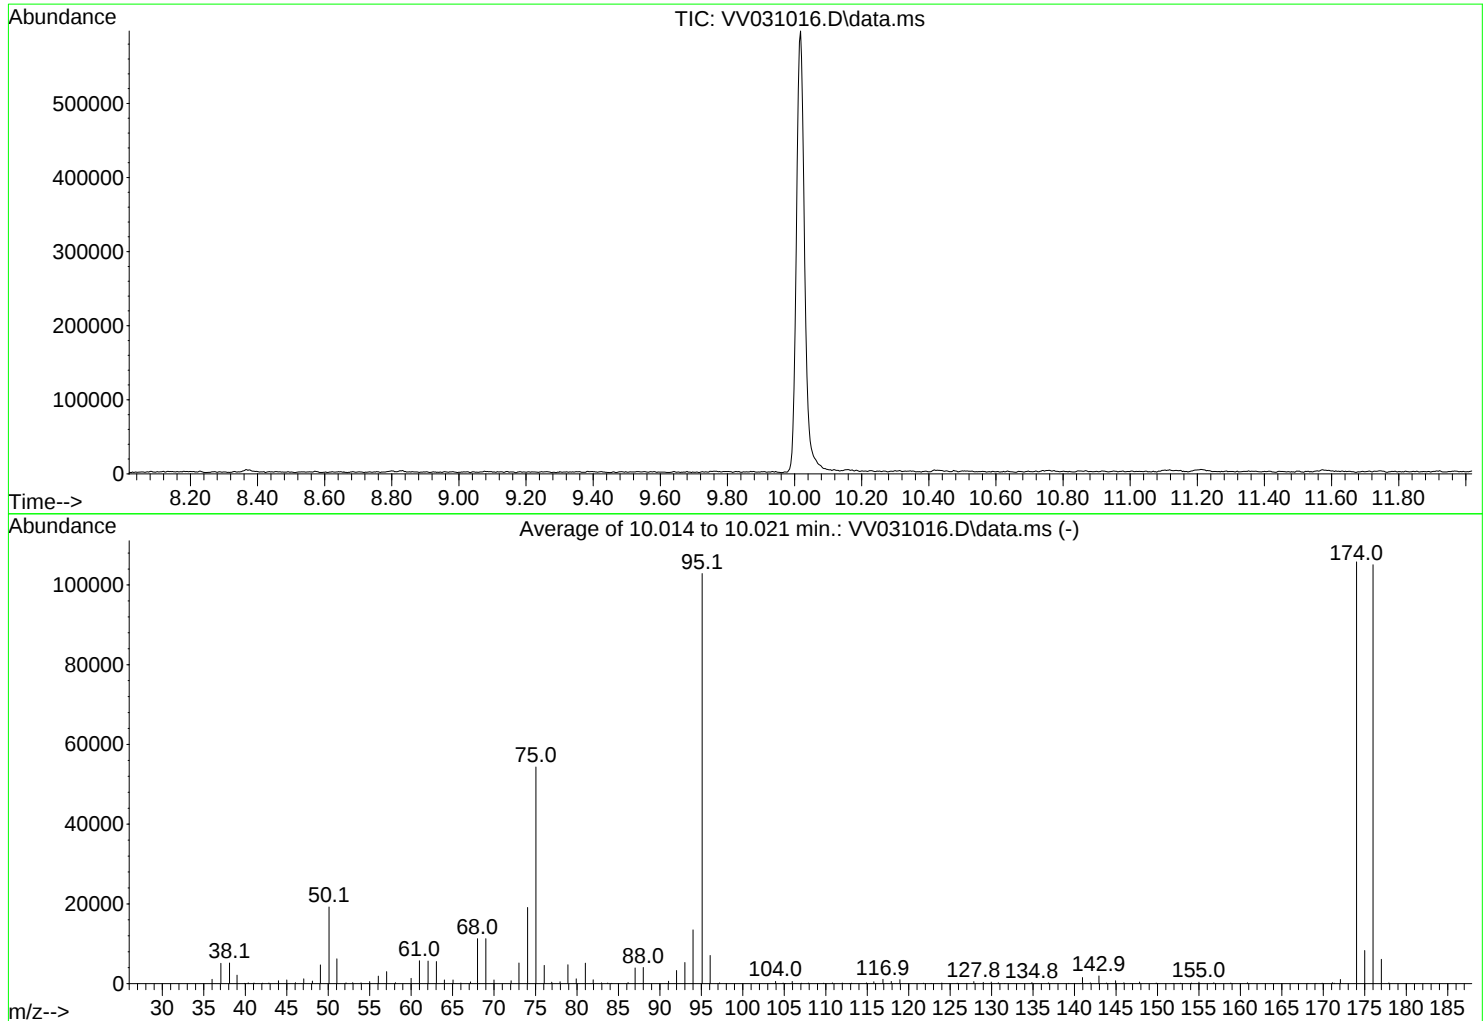

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	19235	PASS
75	95	30	80	52.8	54325	PASS
95	95	100	100	100.0	102861	PASS
96	95	5	9	6.9	7075	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	102.9	105803	PASS
175	174	5	9	7.8	8294	PASS
176	174	95	105	99.3	105085	PASS
177	176	5	10	5.8	6119	PASS

m/z	Abundance
35.60	187.0
36.00	280.0
37.70	177.0
38.60	135.0
39.90	176.0
41.30	106.0
43.30	117.0
44.00	168.0
44.50	110.0
45.20	129.0
51.00	107.0
51.70	108.0
52.30	118.0
57.00	104.0
63.00	105.0
75.00	142.0
76.90	156.0
83.20	106.0
206.90	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB261

m/z	Abundance
36.00	1318.0
37.00	5221.0
38.10	5276.0
39.00	2015.0
39.90	270.0
40.30	219.0
41.10	158.0
42.80	138.0
43.20	146.0
44.10	896.0
45.00	1030.0
46.10	198.0
47.00	1335.0
48.00	711.0
49.10	4883.0
50.10	19552.0
51.10	6229.0
52.10	387.0
52.90	193.0
54.00	172.0
55.00	515.0
56.00	2063.0
57.10	3056.0
58.10	277.0
60.00	1280.0
61.00	5873.0
62.10	5617.0
63.10	5967.0
64.00	858.0
65.00	844.0
66.00	142.0
67.10	472.0
68.00	11594.0
69.00	11470.0
70.00	876.0
72.00	719.0
73.00	5344.0
74.10	19312.0
75.10	54656.0
76.10	4655.0
77.00	613.0
77.90	423.0
78.90	4690.0
79.90	1168.0
81.00	5182.0
81.90	927.0
82.90	255.0
83.70	125.0
86.20	270.0
87.00	3964.0
88.00	4311.0
91.10	564.0
92.00	3327.0
93.00	5303.0
94.00	13375.0
95.10	103992.0
96.00	7096.0
97.20	214.0
103.90	602.0
104.80	257.0
106.00	538.0
107.00	139.0
107.90	184.0
109.70	103.0
110.80	212.0
112.00	176.0
112.90	134.0
114.90	196.0
115.80	497.0
116.90	996.0
117.90	609.0
119.00	989.0
121.80	117.0
122.70	110.0
124.00	125.0
125.90	116.0
127.00	163.0
127.80	483.0
129.00	318.0
129.90	443.0
130.80	248.0
131.60	115.0
134.80	279.0
136.80	201.0
139.30	112.0
140.90	1427.0
141.90	198.0
142.90	1840.0
143.80	169.0
145.00	682.0
146.00	215.0
147.90	452.0

Instrument :
MSVOA_V
ClientSampleId :
BFB261

150.00	159.0
152.80	129.0
154.10	167.0
155.00	394.0
156.80	266.0
158.80	140.0
160.90	213.0
169.10	101.0
169.90	124.0
171.10	389.0
172.10	961.0
174.00	105408.0
175.00	8626.0
176.00	104184.0
177.00	6214.0
177.90	218.0

Instrument :
MSVOA_V
ClientSampleId :
BFB261

m/z	Abundance
36.00	1419.0
37.10	5228.0
38.10	5347.0
39.00	2219.0
39.90	290.0
40.30	204.0
41.10	153.0
42.10	151.0
42.90	154.0
44.00	925.0
45.00	1113.0
46.10	239.0
47.00	1229.0
48.10	658.0
49.10	4867.0
50.10	19672.0
51.10	6516.0
52.10	342.0
52.90	239.0
53.90	219.0
55.00	509.0
56.00	1925.0
57.10	3222.0
58.10	250.0
60.00	1379.0
61.00	5930.0
62.10	5755.0
63.10	5780.0
64.00	956.0
65.10	929.0
66.00	160.0
67.10	463.0
68.00	11654.0
69.00	11622.0
70.00	996.0
72.00	711.0
73.00	5296.0
74.10	19592.0
75.10	55936.0
76.10	4673.0
77.10	482.0
77.90	529.0
78.90	4841.0
79.90	1227.0
81.00	5289.0
82.00	992.0
83.00	181.0
83.70	202.0
84.20	113.0
86.10	279.0
87.00	4054.0
88.00	4204.0
91.00	631.0
92.00	3345.0
93.00	5529.0
94.00	13915.0
95.10	105696.0
96.10	7265.0
97.20	226.0
103.90	615.0
104.90	220.0
106.00	551.0
107.10	122.0
107.90	186.0
109.70	115.0
110.80	194.0
112.00	175.0
113.10	156.0
114.90	199.0
115.80	472.0
116.90	1116.0
117.90	570.0
119.00	1035.0
121.80	134.0
122.70	115.0
124.00	152.0
125.90	138.0
127.00	107.0
127.80	539.0
129.00	318.0
130.00	434.0
130.80	251.0
134.90	305.0
136.80	208.0
139.30	113.0
140.00	123.0
140.90	1547.0
141.90	197.0
142.90	1980.0
143.80	186.0
144.90	722.0
145.90	238.0

Instrument :
MSVOA_V
ClientSampleId :
BFB261

146.80	109.0
147.90	401.0
149.80	159.0
151.90	106.0
152.80	131.0
154.10	187.0
154.90	393.0
156.80	259.0
158.80	160.0
160.80	247.0
168.20	113.0
169.10	126.0
169.80	144.0
171.30	392.0
172.00	1080.0
174.00	109000.0
175.00	8542.0
176.00	108320.0
177.00	6228.0
177.90	229.0

Instrument :
MSVOA_V
ClientSampleId :
BFB261

m/z	Abundance
36.00	1328.0
37.10	4896.0
38.10	4918.0
39.00	2216.0
39.90	245.0
40.40	203.0
41.00	160.0
42.10	181.0
42.90	178.0
44.00	887.0
45.00	1050.0
46.00	242.0
47.10	1066.0
48.20	598.0
49.00	4312.0
50.10	18480.0
51.10	6193.0
52.10	292.0
53.00	262.0
54.00	243.0
55.00	496.0
56.10	1654.0
57.10	3016.0
58.10	186.0
60.00	1324.0
61.00	5446.0
62.00	5645.0
63.10	5204.0
64.00	965.0
65.00	976.0
66.00	144.0
67.20	382.0
68.00	10627.0
69.00	10726.0
70.00	903.0
72.10	684.0
73.00	4875.0
74.00	18392.0
75.10	52808.0
76.00	4465.0
76.90	453.0
78.00	518.0
78.90	4731.0
79.90	1242.0
81.00	5007.0
82.00	949.0
83.00	127.0
83.70	201.0
84.20	133.0
86.10	287.0
87.00	3738.0
88.00	3631.0
91.00	647.0
92.00	3219.0
93.00	5097.0
94.00	13137.0
95.10	98896.0
96.10	6864.0
97.20	218.0
98.00	123.0
104.00	526.0
105.10	184.0
105.90	546.0
107.10	119.0
107.90	156.0
109.80	111.0
110.80	168.0
112.00	196.0
113.10	164.0
114.90	211.0
115.80	444.0
116.90	1093.0
117.90	496.0
118.90	939.0
121.80	100.0
124.00	164.0
125.80	108.0
127.90	571.0
129.00	331.0
130.00	360.0
130.80	198.0
134.80	277.0
136.90	236.0
140.00	126.0
141.00	1576.0
141.90	199.0
143.00	1977.0
143.90	192.0
144.90	766.0
145.90	234.0
146.80	122.0
147.80	369.0

Instrument :
MSVOA_V
ClientSampleId :
BFB261

149.80	148.0
151.90	109.0
152.80	110.0
154.10	177.0
155.10	331.0
156.80	235.0
158.90	167.0
160.80	241.0
168.10	120.0
169.80	159.0
171.10	363.0
172.00	1147.0
174.00	103000.0
175.00	7714.0
176.00	102752.0
177.00	5914.0
177.90	193.0

Instrument :
MSVOA_V
ClientSampleId :
BFB261