

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051723\
 Data File : VV031065.D
 Acq On : 17 May 2023 10:30
 Operator : SY/MD
 Sample : VV0517WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK339

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031065.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	87	rBV	53526	61918	13.48%	1.716%
2	1.536	145	154	167	rBV	58008	75585	16.46%	2.095%
3	2.063	308	318	330	rVB	122460	178966	38.97%	4.960%
4	2.455	429	440	448	rBV4	8248	14881	3.24%	0.412%
5	3.838	858	870	872	rBV	24923	39402	8.58%	1.092%
6	4.259	985	1001	1024	rBV	88566	231553	50.42%	6.418%
7	4.966	1205	1221	1241	rBV2	176582	459257	100.00%	12.729%
8	5.542	1387	1400	1421	rBV	131525	283030	61.63%	7.845%
9	5.838	1485	1492	1497	rBV	3108	4894	1.07%	0.136%
10	5.998	1529	1542	1570	rBV	111597	241348	52.55%	6.690%
11	6.921	1815	1829	1841	rBV	44534	83659	18.22%	2.319%
12	7.249	1919	1931	1950	rBV	187120	342901	74.66%	9.504%
13	7.564	2017	2029	2045	rBV	27525	53372	11.62%	1.479%
14	8.037	2165	2176	2217	rBV	156945	392370	85.44%	10.876%
15	8.371	2273	2280	2281	rBV5	4550	4723	1.03%	0.131%
16	8.793	2400	2411	2435	rBV	201477	353633	77.00%	9.802%
17	10.159	2826	2836	2850	rBV	84209	136144	29.64%	3.774%
18	11.194	3146	3158	3177	rBV	204671	331913	72.27%	9.200%
19	11.567	3262	3274	3291	rBV	188200	313516	68.27%	8.690%
20	13.689	3928	3934	3941	rBV	3790	4768	1.04%	0.132%




Sum of corrected areas: 3607833

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051723\
Data File : VV031065.D
Acq On : 17 May 2023 10:30
Operator : SY/MD
Sample : VV0517WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK339

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

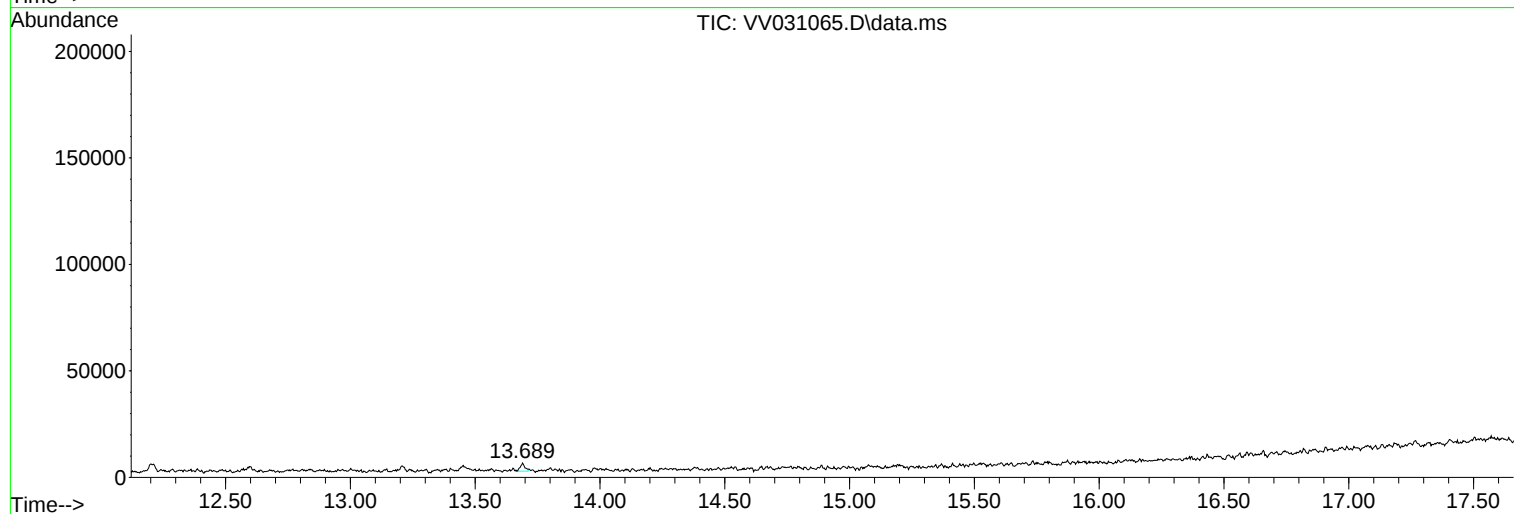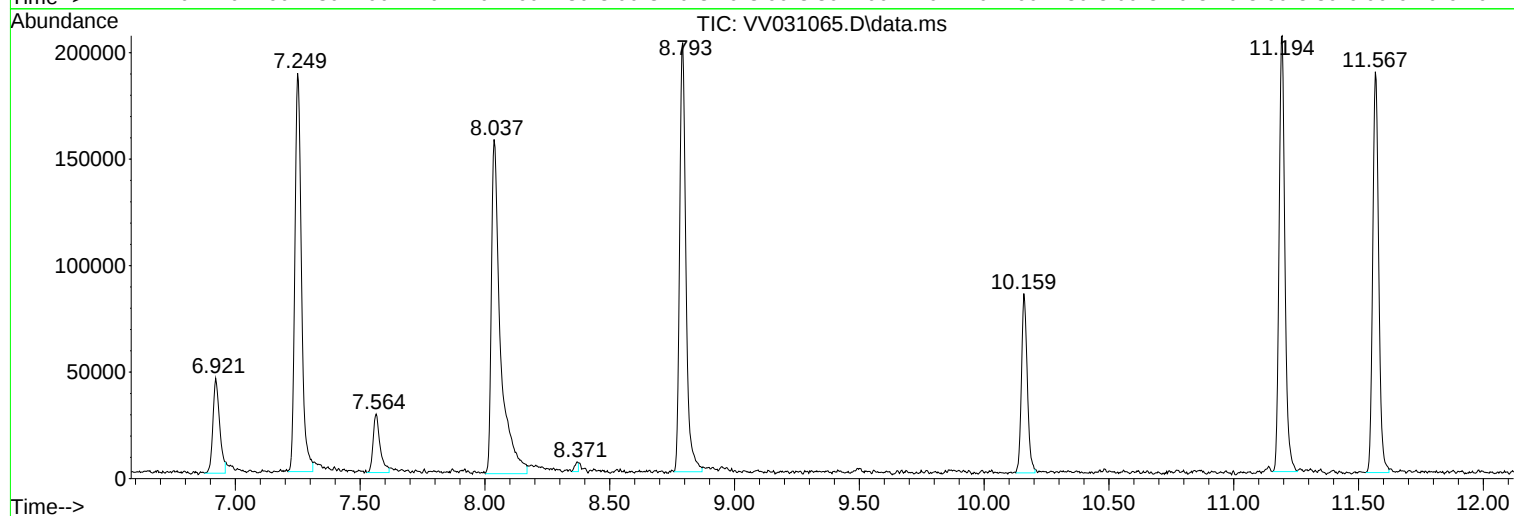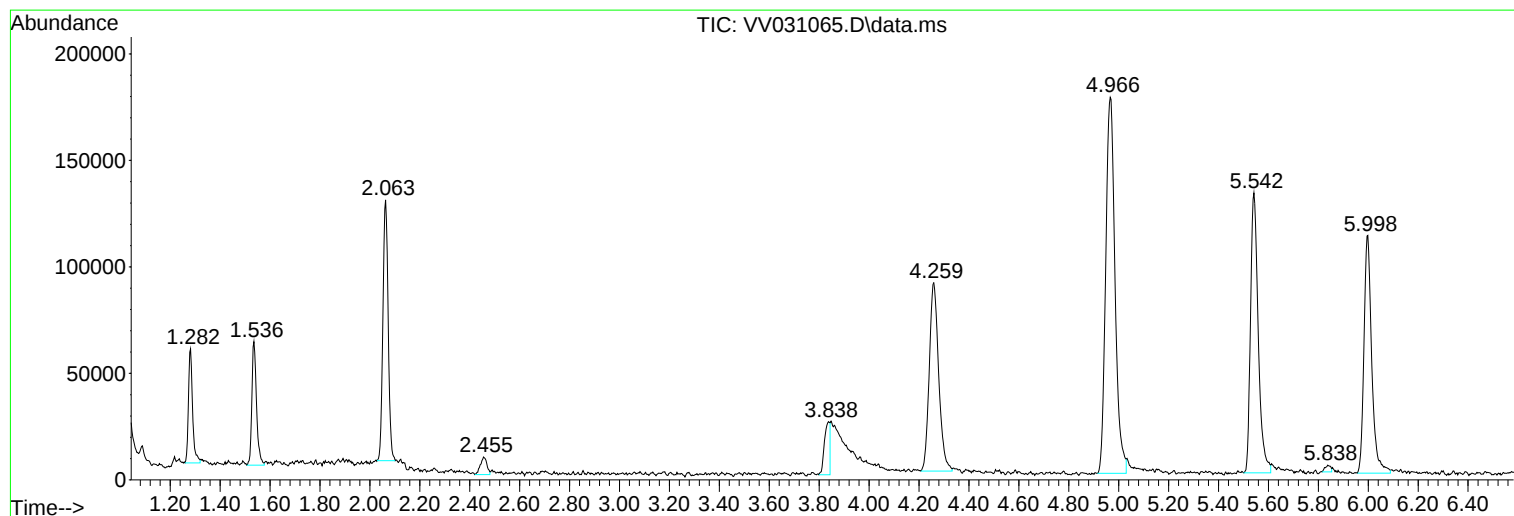

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051723\
Data File : VV031065.D
Acq On : 17 May 2023 10:30
Operator : SY/MD
Sample : VV0517WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK339

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051723\
Data File : VV031065.D
Acq On : 17 May 2023 10:30
Operator : SY/MD
Sample : VV0517WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK339

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc