

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051723\
 Data File : VV031066.D
 Acq On : 17 May 2023 10:57
 Operator : SY/MD
 Sample : 02768-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031066.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	11	14	21	rVB4	7314	7655	1.67%	0.207%
2	1.281	68	75	86	rBV	54942	56902	12.45%	1.542%
3	1.535	146	154	165	rBV	55725	68671	15.02%	1.861%
4	2.063	309	318	333	rBV	118547	172729	37.79%	4.680%
5	2.455	425	440	451	rBV3	13246	27657	6.05%	0.749%
6	3.834	859	869	875	rBV2	25954	56102	12.27%	1.520%
7	4.259	985	1001	1019	rBV2	85462	222534	48.68%	6.030%
8	4.966	1205	1221	1242	rBV2	179644	457119	100.00%	12.387%
9	5.542	1385	1400	1418	rBV	146562	310083	67.83%	8.402%
10	5.995	1525	1541	1559	rBV2	107795	233123	51.00%	6.317%
11	6.921	1817	1829	1845	rBV2	43393	84037	18.38%	2.277%
12	7.249	1919	1931	1950	rBV	189752	340073	74.39%	9.215%
13	7.561	2020	2028	2044	rBV	24938	48238	10.55%	1.307%
14	8.037	2164	2176	2209	rBV	156847	381393	83.43%	10.335%
15	8.792	2397	2411	2433	rBV	223775	390562	85.44%	10.583%
16	10.159	2826	2836	2849	rBV	78952	131231	28.71%	3.556%
17	11.191	3145	3157	3178	rBV	229827	377164	82.51%	10.220%
18	11.567	3260	3274	3289	rBV	196532	317945	69.55%	8.615%
19	12.201	3464	3471	3481	rVB8	4546	7208	1.58%	0.195%




Sum of corrected areas: 3690426

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051723\
Data File : VV031066.D
Acq On : 17 May 2023 10:57
Operator : SY/MD
Sample : 02768-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

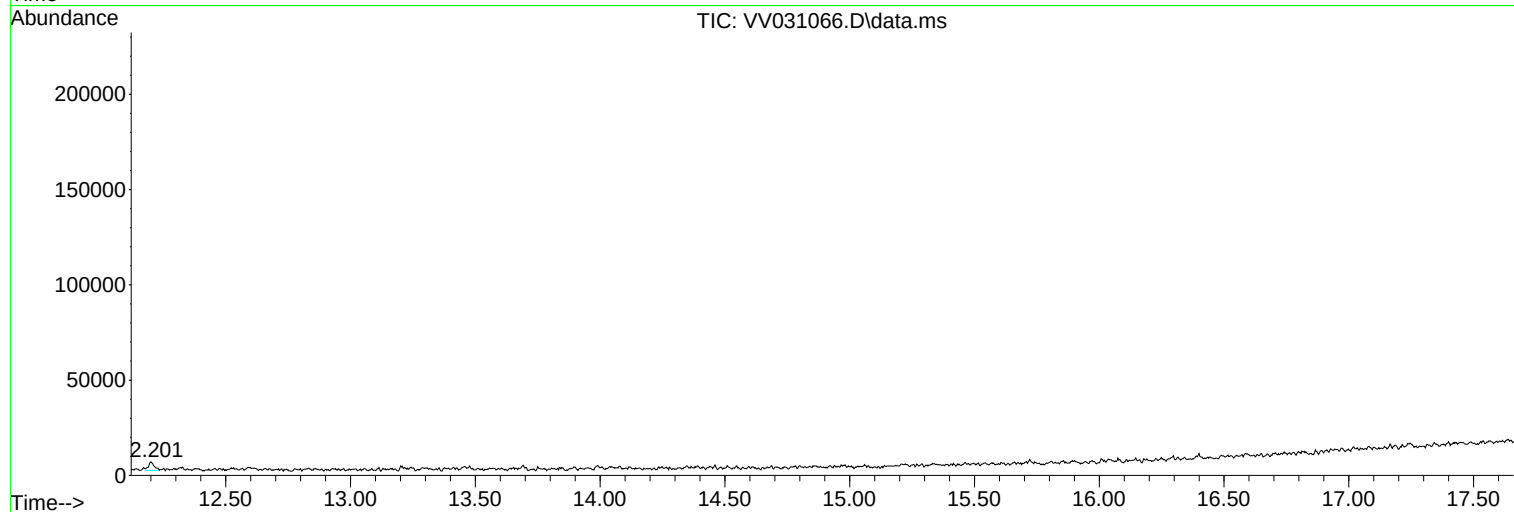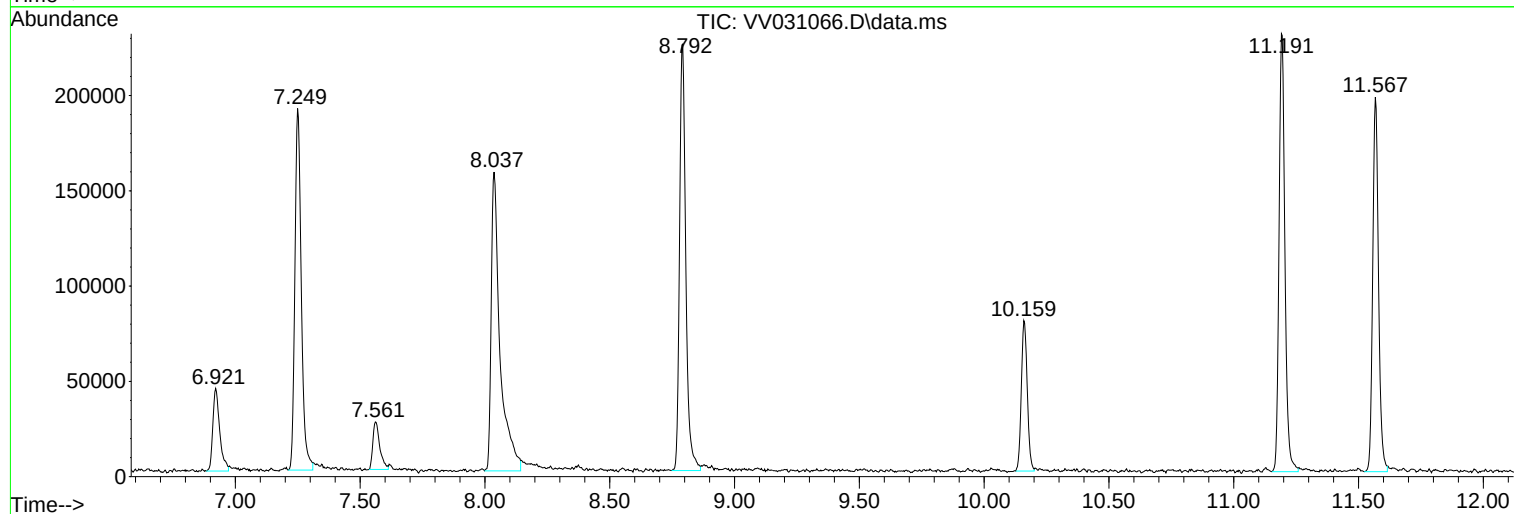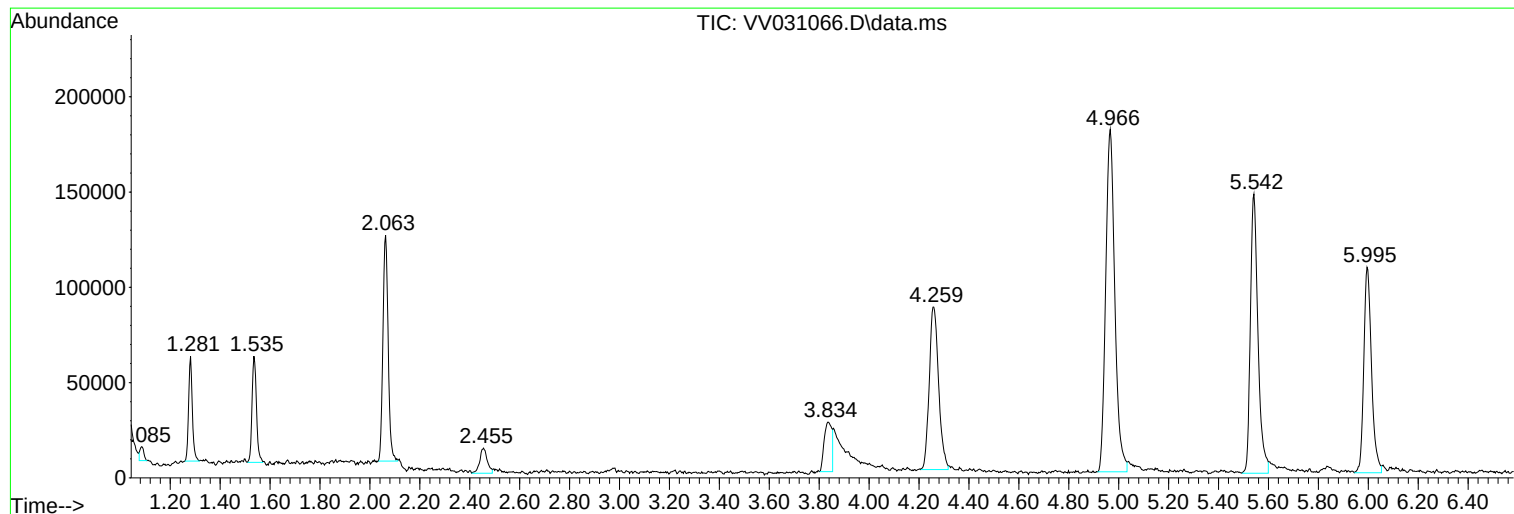

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051723\
Data File : VV031066.D
Acq On : 17 May 2023 10:57
Operator : SY/MD
Sample : 02768-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051723\
Data File : VV031066.D
Acq On : 17 May 2023 10:57
Operator : SY/MD
Sample : 02768-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc