

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051723\
 Data File : VV031079.D
 Acq On : 17 May 2023 17:20
 Operator : SY/MD
 Sample : 02822-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CONM6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031079.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	88	rVB	48135	51779	10.79%	1.288%
2	1.539	148	155	167	rBV	56574	67701	14.10%	1.684%
3	2.066	308	319	331	rBV	107635	159896	33.31%	3.978%
4	3.818	853	864	886	rBV	48841	167837	34.97%	4.176%
5	4.259	985	1001	1024	rBV2	90375	229960	47.91%	5.721%
6	4.966	1205	1221	1244	rBV2	178238	464817	96.84%	11.565%
7	5.542	1389	1400	1423	rBV	147728	307531	64.07%	7.651%
8	5.995	1526	1541	1561	rBV2	110090	239320	49.86%	5.954%
9	6.921	1817	1829	1843	rBV2	44728	87995	18.33%	2.189%
10	7.249	1919	1931	1951	rBV	185954	342858	71.43%	8.530%
11	7.561	2020	2028	2045	rBV2	27764	54384	11.33%	1.353%
12	7.883	2118	2128	2140	rVB3	8210	17300	3.60%	0.430%
13	8.034	2163	2175	2214	rBV	214104	479985	100.00%	11.942%
14	8.793	2398	2411	2436	rBV	230333	400776	83.50%	9.971%
15	10.159	2820	2836	2850	rBV2	92364	152650	31.80%	3.798%
16	10.333	2880	2890	2900	rBV	23515	38683	8.06%	0.962%
17	11.191	3147	3157	3176	rBV	230536	379722	79.11%	9.448%
18	11.503	3242	3254	3261	rBV7	9135	18919	3.94%	0.471%
19	11.567	3263	3274	3289	rVB2	209240	339438	70.72%	8.445%
20	12.204	3463	3472	3484	rBV3	10406	17682	3.68%	0.440%




Sum of corrected areas: 4019233

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051723\
Data File : VV031079.D
Acq On : 17 May 2023 17:20
Operator : SY/MD
Sample : 02822-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONM6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

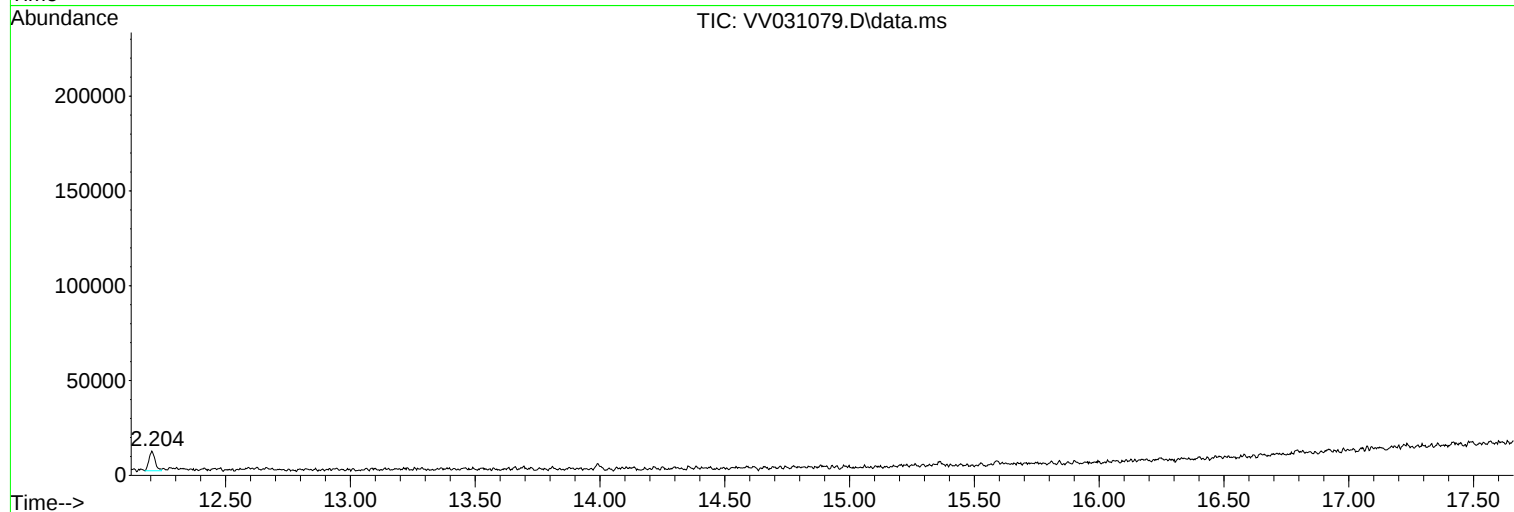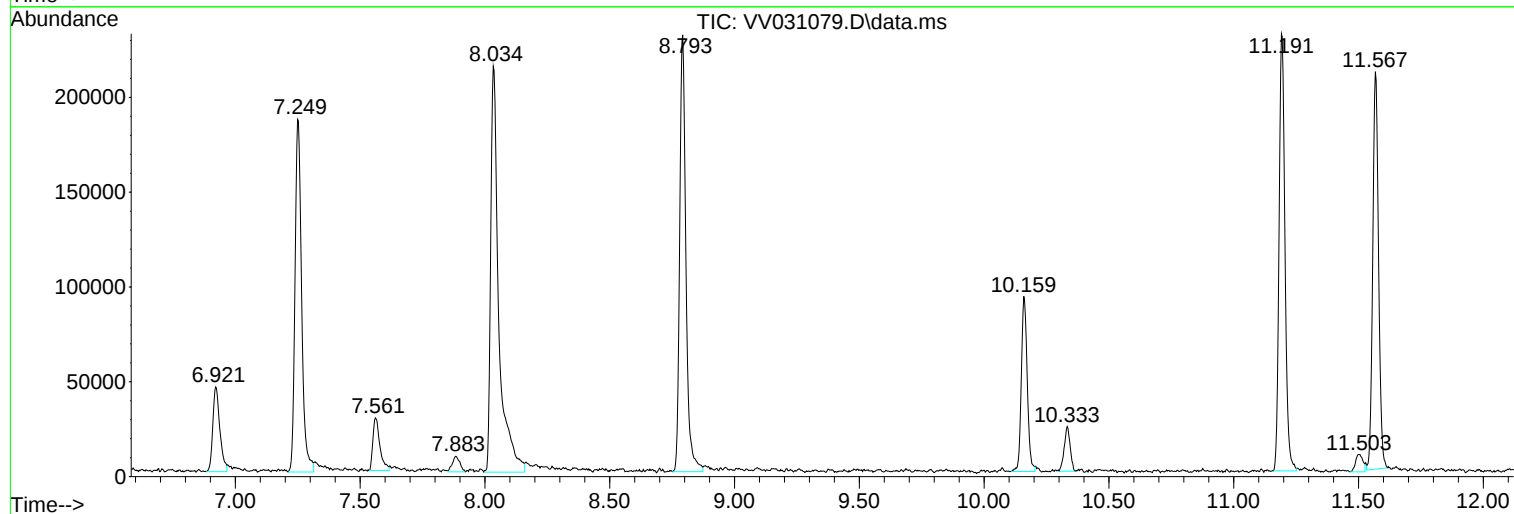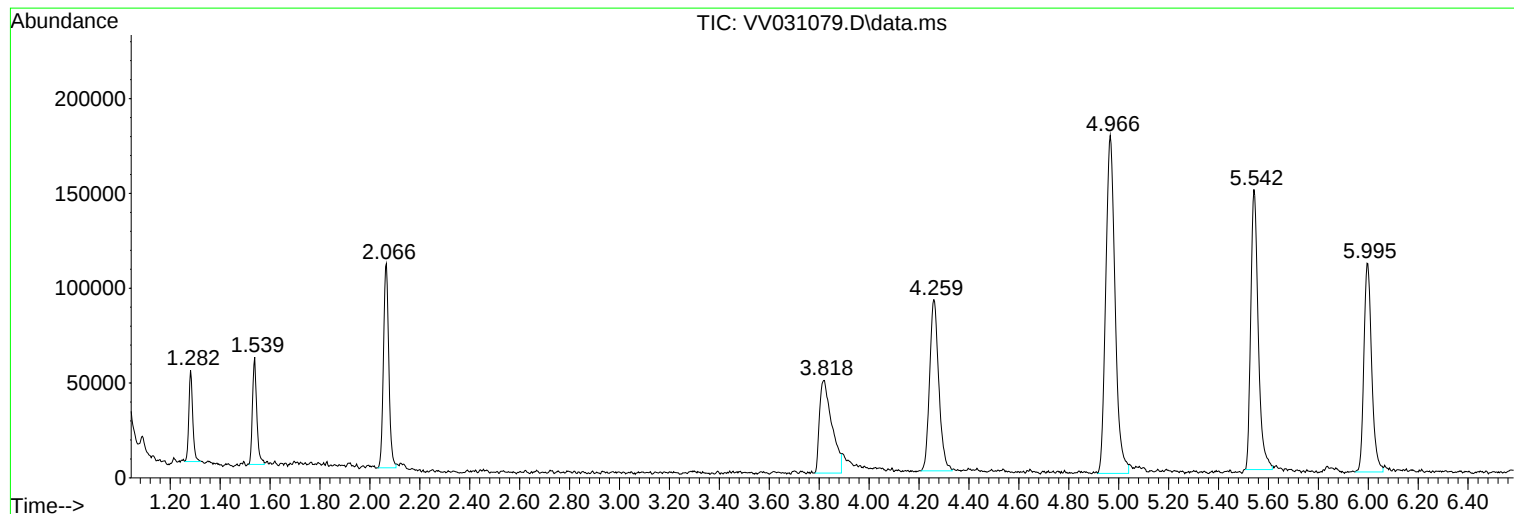

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051723\
Data File : VV031079.D
Acq On : 17 May 2023 17:20
Operator : SY/MD
Sample : 02822-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONM6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051723\
Data File : VV031079.D
Acq On : 17 May 2023 17:20
Operator : SY/MD
Sample : 02822-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONM6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc