
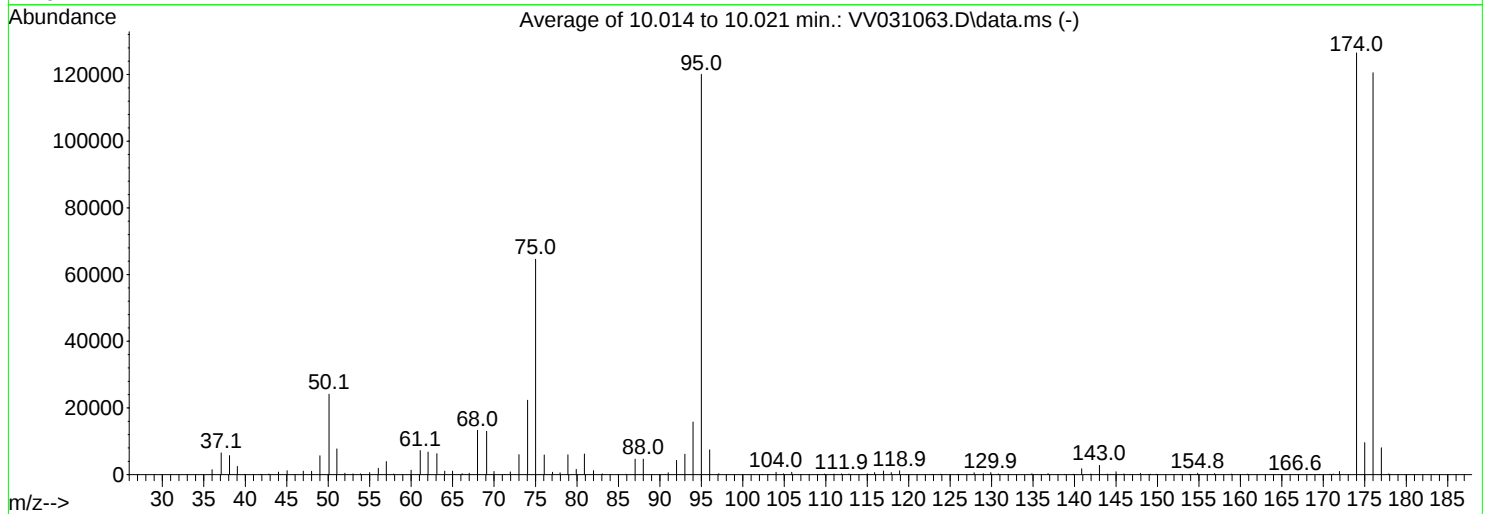


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051723\
 Data File : VV031063.D
 Acq On : 17 May 2023 09:13
 Operator : SY/MD
 Sample : BFB263
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB263

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu May 18 02:47:29 2023

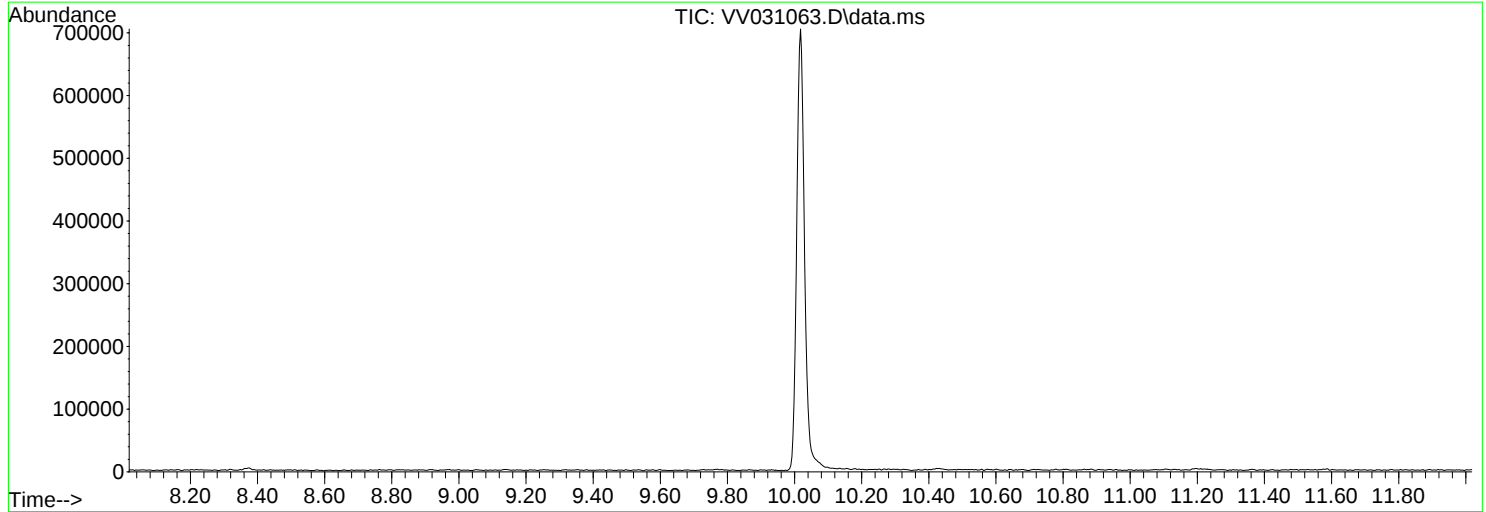

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	24149	PASS
75	95	30	80	53.8	64575	PASS
95	95	100	100	100.0	120045	PASS
96	95	5	9	6.2	7452	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	105.4	126501	PASS
175	174	5	9	7.6	9609	PASS
176	174	95	105	95.3	120557	PASS
177	176	5	10	6.7	8042	PASS

m/z	Abundance
35.30	191.0
36.90	199.0
37.50	139.0
38.90	113.0
40.00	184.0
41.30	118.0
43.10	118.0
43.80	178.0
44.20	212.0
45.80	146.0
47.50	115.0
67.80	106.0
75.10	105.0
288.80	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB263

m/z	Abundance
36.00	1373.0
37.10	6522.0
38.10	5501.0
39.10	2612.0
40.00	266.0
41.00	134.0
42.80	237.0
44.00	1174.0
45.10	1238.0
45.90	178.0
47.00	1039.0
48.00	963.0
49.00	5595.0
50.10	24560.0
51.00	7427.0
52.00	488.0
53.00	224.0
53.90	219.0
55.00	685.0
56.00	1868.0
57.00	3819.0
57.90	179.0
59.00	111.0
60.00	1354.0
61.10	7272.0
62.10	6936.0
63.10	6273.0
64.10	993.0
65.00	1095.0
66.20	234.0
67.00	483.0
68.00	13389.0
69.10	12642.0
70.00	1001.0
71.90	863.0
73.00	5846.0
74.10	22248.0
75.00	64496.0
76.00	5831.0
77.10	620.0
78.00	575.0
78.90	6051.0
79.90	1669.0
80.90	5929.0
82.00	1164.0
83.10	253.0
87.00	4729.0
88.00	4753.0
91.00	657.0
92.00	4240.0
93.00	6189.0
94.00	15593.0
95.00	118704.0
96.00	7651.0
97.10	326.0
104.00	777.0
104.90	302.0
105.90	661.0
107.90	155.0
109.90	208.0
111.00	172.0
111.90	236.0
112.80	148.0
115.00	227.0
115.90	569.0
117.00	1107.0
117.90	626.0
118.90	1114.0
122.80	136.0
123.90	160.0
125.90	107.0
127.90	557.0
129.00	367.0
129.90	602.0
130.80	294.0
134.90	276.0
136.80	364.0
138.70	128.0
139.90	159.0
140.80	1590.0
141.90	199.0
143.00	2636.0
143.90	193.0
145.00	836.0
145.90	270.0
148.00	407.0
149.10	162.0
149.90	147.0
152.80	118.0
154.80	485.0
157.00	330.0
158.90	206.0

Instrument :
MSVOA_V
ClientSampleId :
BFB263

160.90	143.0
166.60	110.0
168.50	102.0
169.60	133.0
171.20	532.0
172.00	940.0
174.00	124128.0
175.00	9288.0
176.00	117992.0
177.00	8130.0
177.90	231.0

Instrument :
MSVOA_V
ClientSampleId :
BFB263

m/z	Abundance
36.00	1587.0
37.10	6741.0
38.10	5835.0
39.10	2615.0
39.90	308.0
40.90	111.0
41.80	113.0
42.80	206.0
44.00	1235.0
45.00	1211.0
46.00	223.0
47.00	1139.0
48.00	1041.0
49.00	5852.0
50.10	24872.0
51.10	8030.0
52.00	450.0
53.00	237.0
53.90	244.0
55.00	638.0
56.00	1975.0
57.00	4070.0
57.90	200.0
58.90	115.0
60.00	1360.0
61.10	7613.0
62.00	6982.0
63.10	6555.0
64.10	1107.0
65.00	1045.0
66.20	290.0
67.00	454.0
68.00	13775.0
69.10	13584.0
70.00	991.0
72.00	873.0
73.00	6184.0
74.00	22880.0
75.00	66728.0
76.10	6188.0
77.00	774.0
77.90	610.0
78.90	6116.0
79.90	1654.0
80.90	6404.0
82.00	1219.0
83.10	271.0
85.90	183.0
87.00	4789.0
88.00	4860.0
91.00	624.0
92.00	4442.0
93.00	6329.0
94.00	16392.0
95.00	123936.0
96.00	7657.0
97.10	314.0
102.40	125.0
104.00	762.0
104.90	289.0
105.90	732.0
107.00	122.0
108.00	119.0
109.80	206.0
111.00	210.0
111.90	274.0
112.80	198.0
115.00	237.0
115.90	630.0
116.90	1155.0
117.90	631.0
118.90	1219.0
119.70	109.0
122.80	117.0
123.90	160.0
125.90	109.0
127.90	598.0
129.00	322.0
129.90	650.0
130.80	287.0
132.00	106.0
134.80	291.0
136.80	370.0
138.80	125.0
139.90	144.0
140.90	1812.0
141.90	186.0
143.00	2854.0
143.90	222.0
145.00	879.0
145.90	273.0
147.90	389.0

Instrument :
MSVOA_V
ClientSampleId :
BFB263

149.20	166.0
149.80	146.0
152.80	112.0
153.90	118.0
154.90	454.0
156.90	338.0
158.90	211.0
160.80	176.0
169.50	119.0
172.00	996.0
174.00	130968.0
175.00	9921.0
176.00	124792.0
177.00	8259.0
177.90	228.0

Instrument :
MSVOA_V
ClientSampleId :
BFB263

m/z	Abundance
36.00	1559.0
37.10	6341.0
38.10	5825.0
39.10	2505.0
39.90	329.0
41.80	157.0
42.90	194.0
44.00	1142.0
45.00	1144.0
46.00	240.0
47.00	1080.0
48.00	1007.0
49.00	5610.0
50.10	23016.0
51.10	7719.0
52.00	414.0
53.00	219.0
53.90	271.0
55.00	515.0
56.10	1910.0
57.00	3907.0
57.90	217.0
58.80	147.0
60.00	1271.0
61.10	6909.0
62.00	6421.0
63.10	6071.0
64.00	1128.0
65.00	999.0
66.10	301.0
67.00	378.0
68.00	12676.0
69.10	12805.0
70.00	972.0
71.30	161.0
72.00	795.0
73.00	5939.0
74.10	21760.0
75.00	62816.0
76.10	5664.0
77.00	761.0
77.90	559.0
78.90	5749.0
79.90	1476.0
80.90	6276.0
82.00	1244.0
83.00	265.0
85.90	214.0
87.00	4439.0
88.00	4346.0
91.00	522.0
92.00	4202.0
93.00	5849.0
94.00	15342.0
95.00	117496.0
96.00	7047.0
97.10	253.0
102.40	133.0
103.10	121.0
104.00	683.0
104.90	262.0
105.90	729.0
107.00	145.0
108.10	101.0
109.80	163.0
111.00	214.0
111.90	240.0
112.80	227.0
115.00	215.0
115.90	626.0
116.90	1140.0
117.90	623.0
118.90	1126.0
119.70	125.0
123.80	121.0
127.90	611.0
129.00	249.0
129.90	691.0
130.80	226.0
132.00	106.0
134.80	289.0
136.80	314.0
138.90	110.0
139.80	151.0
140.90	1913.0
142.00	195.0
143.00	2884.0
144.00	203.0
145.00	852.0
146.00	252.0
146.70	112.0
147.90	396.0

Instrument :
MSVOA_V
ClientSampleId :
BFB263

148.90	143.0
149.20	151.0
149.80	164.0
152.80	114.0
153.80	126.0
154.90	419.0
156.80	335.0
159.00	179.0
160.80	190.0
164.80	100.0
169.30	120.0
170.80	394.0
171.90	1029.0
174.00	124408.0
175.00	9617.0
176.00	118888.0
177.00	7738.0
177.90	213.0

Instrument :
MSVOA_V
ClientSampleId :
BFB263