

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV051820\
 Data File : VV016106.D
 Acq On : 18 May 2020 16:59
 Operator : SY/MD
 Sample : L2655-03DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F21DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM051820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	86	rVB	174645	179033	6.73%	1.477%
2	1.582	146	153	165	rVB	149344	177115	6.65%	1.461%
3	2.126	313	322	352	rVB	285547	424032	15.93%	3.499%
4	2.721	505	507	510	rVB2	462	215	0.01%	0.002%
5	2.920	566	569	572	rBV2	322	256	0.01%	0.002%
6	3.026	599	602	605	rBV2	456	370	0.01%	0.003%
7	3.087	618	621	625	rBV2	372	306	0.01%	0.003%
8	3.135	632	636	640	rBV	392	359	0.01%	0.003%
9	3.171	644	647	650	rVV2	451	288	0.01%	0.002%
10	3.293	680	685	687	rBV	403	224	0.01%	0.002%
11	3.306	687	689	694	rVB2	473	301	0.01%	0.002%
12	3.328	694	696	700	rBV2	315	175	0.01%	0.001%
13	3.357	703	705	708	rVB2	289	114	0.00%	0.001%
14	3.380	710	712	715	rVB2	305	140	0.01%	0.001%
15	3.466	736	739	742	rBV2	287	240	0.01%	0.002%
16	3.508	750	752	755	rVB2	374	184	0.01%	0.002%
17	3.656	795	798	801	rVB	295	148	0.01%	0.001%
18	3.714	812	816	819	rVB3	399	295	0.01%	0.002%
19	3.740	819	824	826	rBV2	292	224	0.01%	0.002%
20	3.791	832	840	845	rBV7	994	1488	0.06%	0.012%
21	3.852	858	859	864	rVB	259	118	0.00%	0.001%
22	3.933	873	884	918	rBV	70559	257648	9.68%	2.126%
23	4.380	1006	1023	1059	rBV	199065	525083	19.72%	4.332%
24	4.663	1106	1111	1113	rBV2	379	317	0.01%	0.003%
25	4.685	1115	1118	1119	rBV	617	287	0.01%	0.002%
26	4.791	1144	1151	1155	rBV5	385	556	0.02%	0.005%
27	4.859	1163	1172	1173	rBV3	1333	1371	0.05%	0.011%
28	4.901	1183	1185	1191	rVB	421	351	0.01%	0.003%
29	4.926	1191	1193	1196	rBV3	263	207	0.01%	0.002%
30	4.978	1205	1209	1210	rBV	306	180	0.01%	0.001%
31	5.074	1221	1239	1251	rBV2	504930	1302503	48.93%	10.746%
32	5.312	1309	1313	1317	rBV4	599	586	0.02%	0.005%
33	5.405	1341	1342	1347	rBV2	418	218	0.01%	0.002%
34	5.431	1347	1350	1352	rBV2	293	219	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV051820\
 Data File : VV016106.D
 Acq On : 18 May 2020 16:59
 Operator : SY/MD
 Sample : L2655-03DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F21DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM051820WMA.M
 Title : VOC Analysis

35	5.547	1384	1386	1388	rBV	309	136	0.01%	0.001%
36	5.643	1402	1416	1440	rBV	399282	793038	29.79%	6.543%
37	6.000	1525	1527	1531	rBV2	391	265	0.01%	0.002%
38	6.097	1541	1557	1579	rBV	295626	597896	22.46%	4.933%
39	6.328	1627	1629	1633	rBV2	169	114	0.00%	0.001%
40	6.396	1647	1650	1653	rBV4	496	268	0.01%	0.002%
41	6.457	1667	1669	1671	rVV2	317	116	0.00%	0.001%
42	6.476	1671	1675	1676	rVV2	231	131	0.00%	0.001%
43	6.531	1689	1692	1693	rBV	298	159	0.01%	0.001%
44	6.556	1697	1700	1702	rBV2	247	192	0.01%	0.002%
45	6.656	1726	1731	1733	rBV2	856	828	0.03%	0.007%
46	6.794	1772	1774	1778	rBV2	333	200	0.01%	0.002%
47	6.859	1791	1794	1797	rBV	210	159	0.01%	0.001%
48	6.907	1805	1809	1810	rBV	218	161	0.01%	0.001%
49	6.926	1814	1815	1819	rVB	266	145	0.01%	0.001%
50	6.945	1819	1821	1823	rBV	233	111	0.00%	0.001%
51	7.010	1830	1841	1862	rBV	162429	294720	11.07%	2.432%
52	7.193	1896	1898	1899	rBV	407	201	0.01%	0.002%
53	7.341	1930	1944	1966	rBV	601358	1051728	39.51%	8.677%
54	7.643	2028	2038	2057	rBV	118781	200254	7.52%	1.652%
55	7.817	2087	2092	2095	rBV4	666	695	0.03%	0.006%
56	7.891	2112	2115	2118	rVB2	410	234	0.01%	0.002%
57	7.907	2118	2120	2123	rVB2	301	141	0.01%	0.001%
58	7.952	2131	2134	2135	rBV2	532	276	0.01%	0.002%
59	8.010	2151	2152	2156	rVB	723	287	0.01%	0.002%
60	8.032	2156	2159	2160	rBV	228	113	0.00%	0.001%
61	8.119	2175	2186	2215	rBV	258535	538420	20.23%	4.442%
62	8.402	2271	2274	2276	rBV2	487	239	0.01%	0.002%
63	8.569	2322	2326	2327	rVV2	580	281	0.01%	0.002%
64	8.598	2331	2335	2339	rBV2	351	367	0.01%	0.003%
65	8.685	2359	2362	2366	rVB	477	385	0.01%	0.003%
66	8.707	2366	2369	2371	rBV2	430	232	0.01%	0.002%
67	8.720	2371	2373	2376	rVV2	332	176	0.01%	0.001%
68	8.772	2386	2389	2392	rBV3	309	190	0.01%	0.002%
69	8.804	2396	2399	2401	rBV2	340	204	0.01%	0.002%
70	8.875	2409	2421	2424	rBV	657280	933343	35.06%	7.701%
71	9.161	2505	2510	2513	rBV2	416	462	0.02%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV051820\
 Data File : VV016106.D
 Acq On : 18 May 2020 16:59
 Operator : SY/MD
 Sample : L2655-03DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F21DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM051820WMA.M
 Title : VOC Analysis

72	9.187	2516	2518	2523	rVB2	601	281	0.01%	0.002%
73	9.219	2523	2528	2533	rBV4	555	525	0.02%	0.004%
74	9.309	2551	2556	2558	rBV3	437	323	0.01%	0.003%
75	9.434	2592	2595	2597	rBV2	236	137	0.01%	0.001%
76	9.701	2676	2678	2680	rBV2	284	130	0.00%	0.001%
77	9.759	2694	2696	2700	rVB2	349	193	0.01%	0.002%
78	9.788	2700	2705	2706	rBV	355	218	0.01%	0.002%
79	9.913	2742	2744	2747	rVB	416	169	0.01%	0.001%
80	9.932	2747	2750	2753	rBV	313	210	0.01%	0.002%
81	9.952	2753	2756	2761	rVV3	409	296	0.01%	0.002%
82	10.238	2833	2845	2860	rBV	359436	561307	21.09%	4.631%
83	10.354	2878	2881	2884	rBV3	423	342	0.01%	0.003%
84	10.399	2891	2895	2899	rBV2	720	708	0.03%	0.006%
85	10.563	2944	2946	2952	rVB3	496	399	0.01%	0.003%
86	10.727	2993	2997	2999	rBV2	389	260	0.01%	0.002%
87	11.013	3083	3086	3090	rBV2	413	262	0.01%	0.002%
88	11.206	3135	3146	3156	rBV	108406	168403	6.33%	1.389%
89	11.276	3156	3168	3169	rBV	726751	920017	34.56%	7.591%
90	11.662	3270	3288	3312	rBV2	1218844	2662098	100.00%	21.964%
91	11.865	3348	3351	3353	rBV2	444	348	0.01%	0.003%
92	12.170	3444	3446	3447	rBV2	387	143	0.01%	0.001%
93	12.431	3520	3527	3529	rBV5	1337	1487	0.06%	0.012%
94	12.604	3578	3581	3583	rBV2	514	367	0.01%	0.003%
95	12.672	3598	3602	3610	rVB5	2172	2884	0.11%	0.024%
96	13.141	3746	3748	3750	rBV	513	328	0.01%	0.003%
97	13.286	3781	3793	3810	rBV	244267	377333	14.17%	3.113%
98	13.768	3933	3943	3959	rVB	72845	114208	4.29%	0.942%
99	14.177	4066	4070	4072	rBV4	793	593	0.02%	0.005%
100	15.424	4451	4458	4467	rVB3	9591	14328	0.54%	0.118%


Sum of corrected areas: 12120315

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV051820\
Data File : VV016106.D
Acq On : 18 May 2020 16:59
Operator : SY/MD
Sample : L2655-03DL 5X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F21DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM051820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

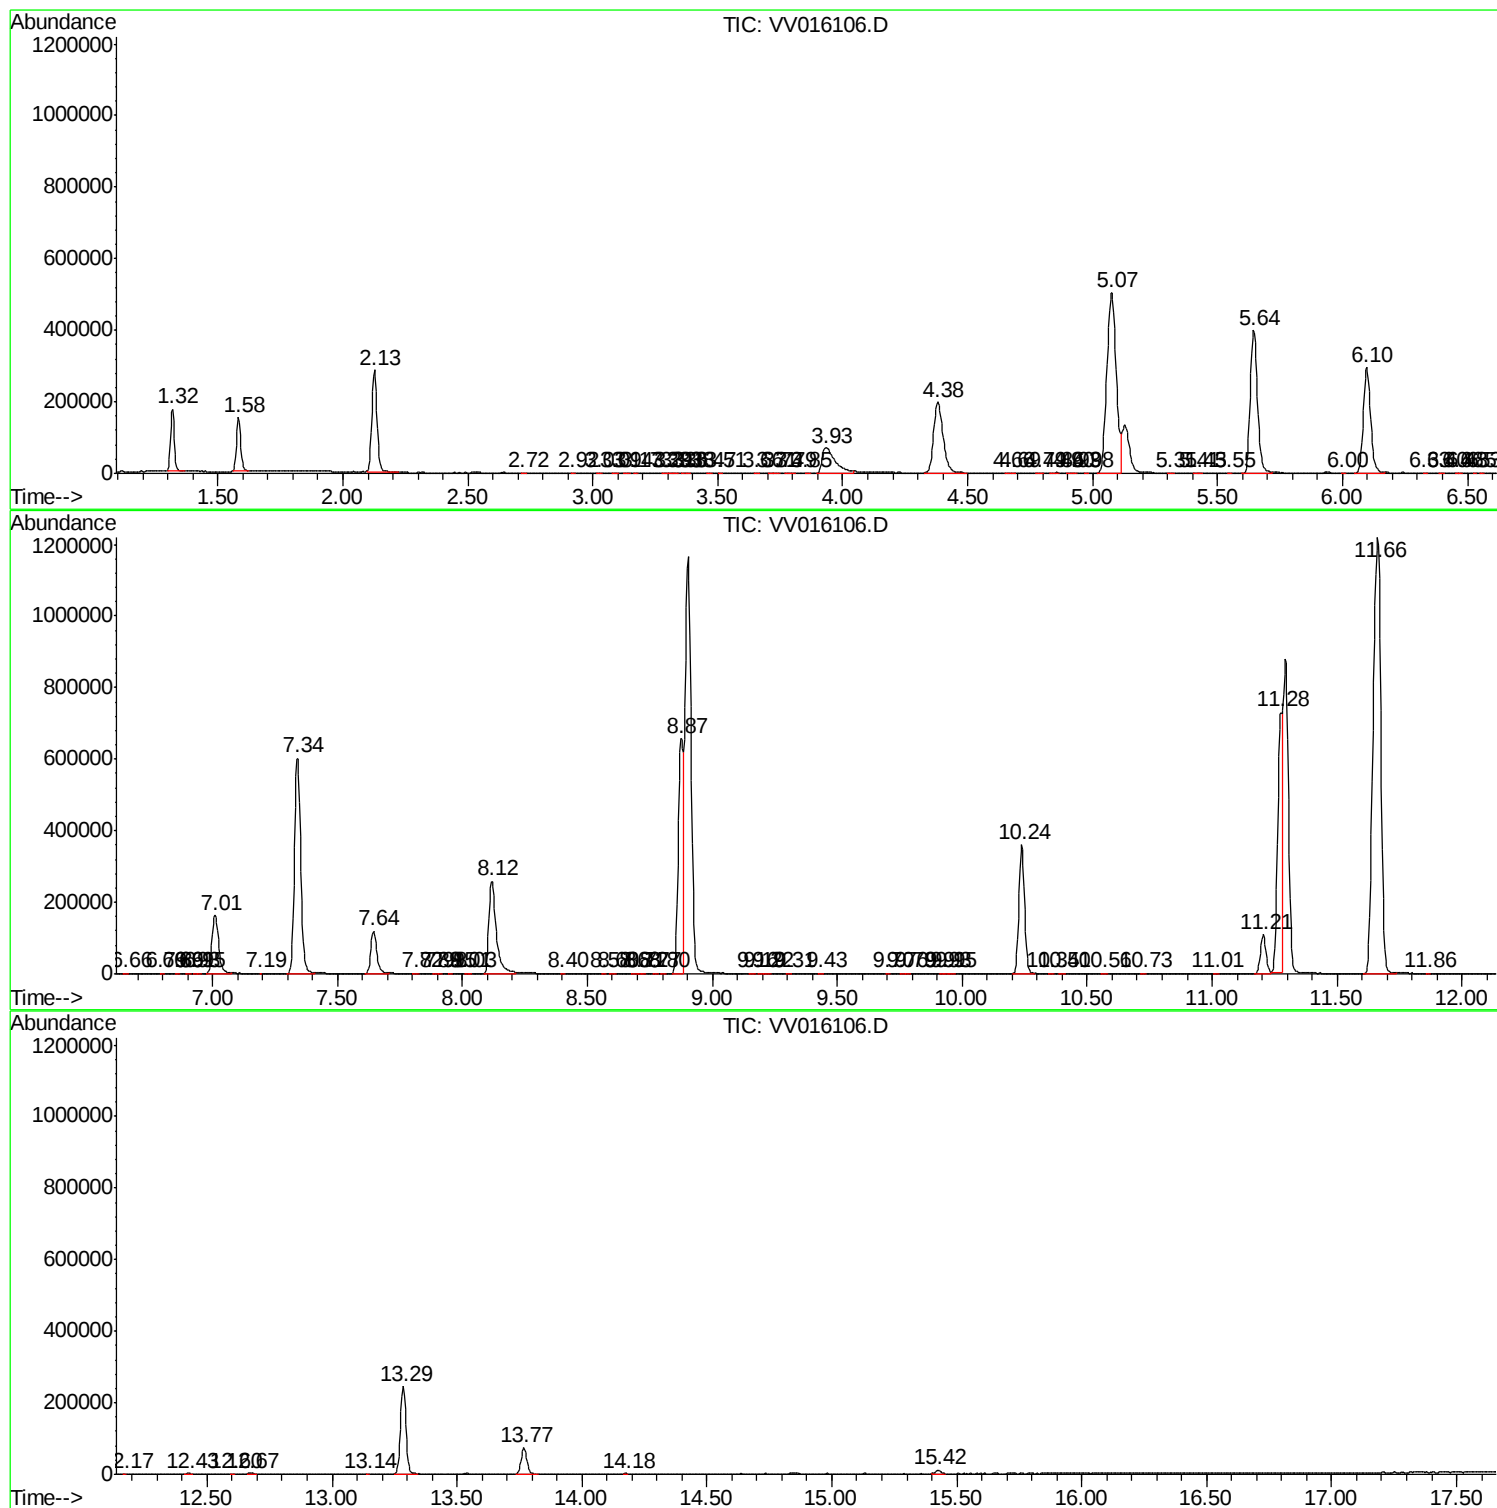

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV051820\
Data File : VV016106.D
Acq On : 18 May 2020 16:59
Operator : SY/MD
Sample : L2655-03DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F21DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM051820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV051820\
Data File : VV016106.D
Acq On : 18 May 2020 16:59
Operator : SY/MD
Sample : L2655-03DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F21DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM051820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc