


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV051820\
 Data File : VV016089.D
 Acq On : 18 May 2020 08:57
 Operator : SY/MD
 Sample : BFB77
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB77

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM051820WMA.M
 Title : VOC Analysis
 Last Update : Tue May 19 04:04:01 2020

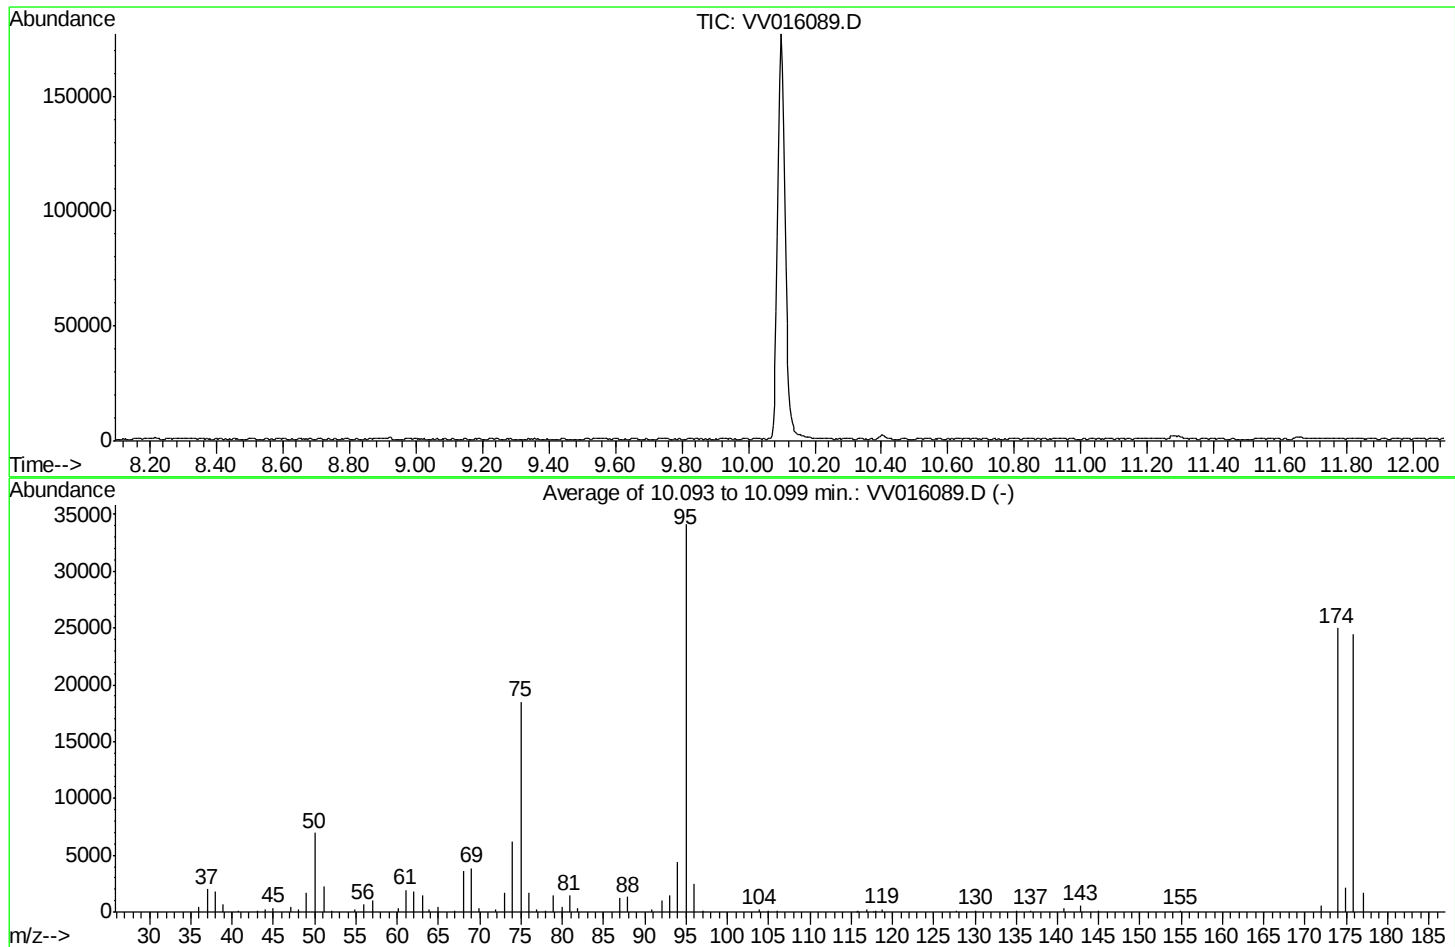

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	6961	PASS
75	95	30	80	54.3	18536	PASS
95	95	100	100	100.0	34122	PASS
96	95	5	9	7.3	2479	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.2	24973	PASS
175	174	5	9	8.4	2100	PASS
176	174	95	101	98.1	24493	PASS
177	176	5	9	7.0	1712	PASS

m/z	Abundance
35.90	478.0
37.00	1993.0
38.00	1689.0
39.00	786.0
39.80	332.0
40.80	116.0
44.00	695.0
45.00	377.0
47.00	448.0
47.90	250.0
49.00	1514.0
50.00	6482.0
51.10	2063.0
52.00	142.0
54.80	209.0
55.90	666.0
57.00	1044.0
60.10	386.0
61.00	1812.0
61.90	1744.0
63.00	1316.0
63.90	210.0
64.90	437.0
67.00	133.0
68.00	3265.0
69.00	3758.0
69.90	255.0
71.90	165.0
73.00	1618.0
74.00	5734.0
75.00	17352.0
76.00	1579.0
76.90	241.0
77.90	142.0
78.90	1326.0
80.00	395.0
80.90	1400.0
81.80	297.0
86.90	1069.0
87.90	1229.0
91.00	238.0
92.00	891.0
93.00	1436.0
94.00	4142.0
95.00	31848.0
96.00	2427.0
103.90	196.0
105.00	135.0
106.00	130.0
115.70	123.0
115.90	124.0
116.90	217.0
118.00	115.0
118.70	232.0
130.20	115.0
136.70	102.0
140.90	352.0
142.90	478.0
154.90	154.0
171.90	502.0
173.90	22728.0
174.90	1929.0
175.90	21744.0
177.00	1628.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

m/z	Abundance
35.90	487.0
37.00	2042.0
38.00	1952.0
39.00	844.0
39.90	296.0
40.80	136.0
43.00	122.0
44.00	711.0
44.90	382.0
47.10	482.0
47.90	249.0
49.00	1654.0
50.00	7139.0
51.00	2369.0
52.00	120.0
54.80	252.0
55.90	677.0
57.00	1089.0
60.00	410.0
61.00	1967.0
61.90	1810.0
63.00	1472.0
63.90	222.0
64.90	452.0
67.00	170.0
68.00	3647.0
69.00	3999.0
70.00	331.0
71.90	192.0
73.00	1822.0
74.00	6367.0
75.00	19312.0
76.00	1767.0
77.00	255.0
77.90	159.0
78.90	1476.0
80.00	443.0
80.90	1512.0
81.90	323.0
86.90	1245.0
87.90	1388.0
90.90	253.0
92.00	1023.0
93.00	1572.0
94.00	4562.0
95.00	35320.0
96.00	2555.0
97.00	122.0
103.90	209.0
105.00	134.0
106.00	146.0
115.90	139.0
116.80	252.0
117.90	107.0
118.80	254.0
127.70	114.0
130.10	138.0
135.00	106.0
136.80	133.0
140.80	373.0
142.90	546.0
144.90	114.0
154.90	155.0
171.90	585.0
173.90	25880.0
174.90	2175.0
175.90	25136.0
177.00	1805.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

m/z	Abundance
35.90	439.0
37.00	1949.0
38.00	2065.0
39.00	906.0
39.90	307.0
40.80	140.0
43.00	138.0
44.00	687.0
45.00	341.0
47.10	465.0
48.00	250.0
49.00	1774.0
50.00	7264.0
51.00	2390.0
54.90	260.0
55.90	671.0
57.00	1031.0
60.00	360.0
61.00	1996.0
62.00	1822.0
63.00	1503.0
63.90	195.0
64.90	392.0
67.00	201.0
68.00	3873.0
69.00	3763.0
70.00	353.0
71.90	204.0
73.00	1772.0
74.00	6490.0
75.00	18944.0
76.00	1774.0
77.00	247.0
77.90	167.0
78.90	1460.0
79.90	455.0
80.80	1456.0
81.90	354.0
86.90	1366.0
88.00	1350.0
90.80	269.0
92.00	1101.0
92.90	1529.0
94.00	4535.0
95.00	35200.0
96.00	2457.0
97.00	112.0
103.90	214.0
106.00	151.0
115.80	137.0
116.80	250.0
117.70	123.0
118.90	288.0
127.70	149.0
130.00	146.0
135.00	103.0
136.70	145.0
140.90	377.0
142.80	540.0
144.90	118.0
154.90	125.0
171.90	636.0
173.90	26312.0
174.90	2197.0
175.90	26600.0
177.00	1705.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

Scan 2790 (10.061 min): VV016089.D
BFB77

m/z	Abundance
38.10	101.0
38.90	120.0
39.90	438.0
42.10	111.0
43.90	489.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77