


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051822\
 Data File : VV025926.D
 Acq On : 18 May 2022 09:30
 Operator : SY/MD
 Sample : BFB201
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB201

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM051822.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu May 19 07:42:58 2022

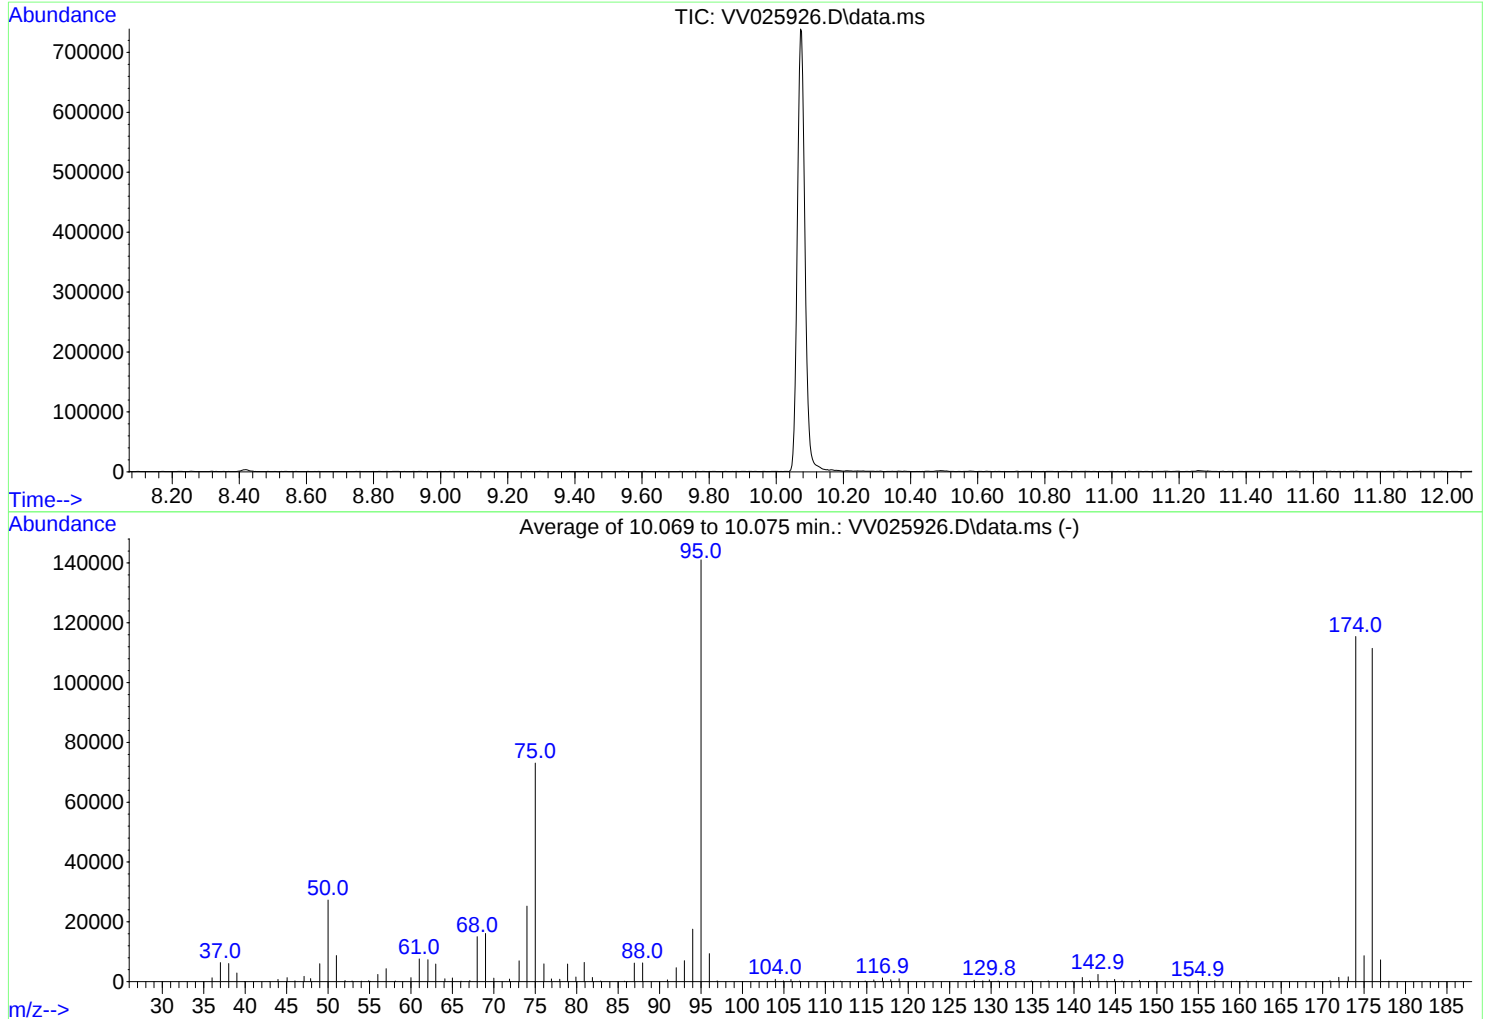

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	27317	PASS
75	95	30	80	51.8	73101	PASS
95	95	100	100	100.0	141056	PASS
96	95	5	9	6.7	9383	PASS
173	174	0.00	2	1.4	1585	PASS
174	95	50	120	81.8	115435	PASS
175	174	5	9	7.5	8671	PASS
176	174	95	101	96.5	111451	PASS
177	176	5	9	6.5	7297	PASS

m/z	Abundance
35.70	105.0
40.00	291.0
43.90	511.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201

m/z	Abundance
36.00	1258.0
37.00	5984.0
38.00	5975.0
39.00	2693.0
39.90	298.0
42.90	123.0
44.00	1151.0
45.10	1365.0
46.00	263.0
47.10	1666.0
47.90	968.0
49.00	5760.0
50.00	25944.0
51.00	8347.0
52.10	380.0
52.90	206.0
54.00	110.0
54.90	502.0
56.00	2391.0
57.00	4041.0
58.10	187.0
60.00	1289.0
61.00	7372.0
62.00	6883.0
63.00	5683.0
64.10	947.0
65.00	1204.0
66.10	146.0
67.10	354.0
68.00	14428.0
69.00	15171.0
70.00	1052.0
71.90	784.0
73.00	6648.0
74.00	23880.0
75.00	69632.0
76.10	5815.0
76.90	875.0
77.90	716.0
78.90	5697.0
79.90	1424.0
80.90	6243.0
81.90	1295.0
82.90	225.0
86.10	173.0
87.00	5910.0
87.90	5948.0
91.00	576.0
92.00	4270.0
93.00	6737.0
94.00	16480.0
95.00	132672.0
96.00	8938.0
97.00	263.0
104.00	756.0
105.00	248.0
105.80	672.0
106.90	190.0
109.80	143.0
111.00	189.0
111.80	149.0
114.80	156.0
115.80	573.0
116.90	1268.0
117.90	698.0
118.90	928.0
127.90	516.0
129.00	249.0
129.80	509.0
130.80	223.0
134.80	229.0
136.90	271.0
139.80	180.0
141.00	1315.0
141.90	231.0
142.90	2273.0
144.00	129.0
144.90	810.0
145.80	166.0
146.10	196.0
147.90	387.0
149.90	157.0
153.00	118.0
153.80	105.0
155.00	267.0
157.00	265.0
159.00	177.0
160.80	193.0
170.90	282.0
171.90	1281.0
173.10	1455.0
174.00	105008.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201

175.00	7876.0
176.00	102328.0
177.00	6846.0
178.00	130.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201

m/z	Abundance
36.00	1325.0
37.00	6508.0
38.00	6228.0
39.00	2942.0
39.90	357.0
44.00	1303.0
45.00	1352.0
46.00	263.0
47.10	1842.0
47.90	1038.0
49.00	6094.0
50.00	28136.0
51.00	9038.0
52.00	370.0
52.90	213.0
54.10	149.0
54.90	455.0
56.00	2487.0
57.00	4477.0
58.10	215.0
60.00	1393.0
61.00	7911.0
62.10	7626.0
63.00	6084.0
64.10	1008.0
65.00	1223.0
66.10	153.0
67.10	418.0
68.00	15539.0
69.00	16752.0
70.00	1230.0
71.90	873.0
73.00	7302.0
74.00	26032.0
75.00	75800.0
76.00	6138.0
77.00	943.0
77.90	857.0
78.90	6018.0
79.90	1606.0
80.90	6677.0
81.90	1447.0
82.90	251.0
85.80	211.0
86.90	6357.0
88.00	6412.0
91.00	621.0
92.00	4864.0
93.00	7323.0
94.00	18160.0
95.00	145920.0
96.00	9720.0
97.00	281.0
104.00	859.0
104.90	253.0
105.90	725.0
106.90	202.0
107.90	108.0
109.90	130.0
111.00	181.0
111.80	174.0
114.80	203.0
115.80	637.0
116.90	1256.0
117.90	684.0
118.90	1044.0
128.00	537.0
129.00	257.0
129.80	595.0
130.90	220.0
134.90	280.0
136.90	266.0
139.80	155.0
141.00	1443.0
141.90	268.0
142.90	2519.0
144.00	161.0
144.90	817.0
145.80	206.0
146.10	196.0
147.90	426.0
149.80	146.0
151.70	100.0
153.00	133.0
154.90	345.0
157.00	333.0
159.00	170.0
160.90	198.0
170.90	304.0
172.00	1464.0
173.10	1630.0
174.00	119096.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201

175.00	8999.0
176.00	115584.0
177.00	7521.0
178.00	149.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201

m/z	Abundance
36.00	1269.0
37.00	6585.0
38.00	5934.0
39.00	2993.0
39.90	388.0
44.00	1363.0
45.00	1260.0
46.00	232.0
47.10	1766.0
47.90	984.0
49.00	6085.0
50.00	27872.0
51.00	8841.0
52.00	354.0
52.90	204.0
54.10	183.0
55.10	389.0
56.00	2312.0
57.00	4480.0
58.10	220.0
60.00	1405.0
61.00	7599.0
62.00	7451.0
63.00	5902.0
64.10	974.0
65.00	1297.0
65.90	178.0
67.10	446.0
68.00	15154.0
69.00	16400.0
70.00	1225.0
71.90	905.0
73.10	6897.0
74.00	25816.0
75.00	73872.0
76.00	5929.0
77.00	1006.0
78.00	874.0
78.90	5893.0
79.90	1619.0
80.90	6315.0
81.90	1483.0
82.90	228.0
85.80	230.0
87.00	6374.0
88.00	6379.0
90.90	652.0
92.00	4818.0
93.00	6946.0
94.00	18064.0
95.00	144576.0
96.00	9490.0
96.90	243.0
103.90	795.0
104.90	269.0
105.90	687.0
106.90	203.0
109.90	118.0
110.90	155.0
111.90	154.0
113.00	103.0
114.80	220.0
115.90	656.0
116.90	1134.0
117.90	632.0
118.90	981.0
127.90	454.0
129.00	276.0
129.80	677.0
130.90	203.0
134.90	296.0
136.90	259.0
139.80	110.0
141.00	1409.0
141.90	283.0
142.90	2479.0
143.80	157.0
144.90	686.0
145.80	220.0
147.10	116.0
147.90	424.0
148.80	113.0
149.70	124.0
151.70	108.0
153.00	121.0
154.90	360.0
157.00	354.0
159.00	138.0
160.90	198.0
170.90	326.0
172.00	1599.0
173.10	1670.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201

174.00	122200.0
175.00	9137.0
176.00	116440.0
177.00	7524.0
178.00	193.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201