

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051823\
 Data File : VV031086.D
 Acq On : 18 May 2023 10:31
 Operator : SY/MD
 Sample : VV0518WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK340

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031086.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.088	11	15	25	rVB	11596	11286	2.46%	0.314%
2	1.281	69	75	85	rBV	51740	54614	11.91%	1.521%
3	1.539	148	155	169	rVB	56533	68718	14.99%	1.914%
4	2.063	307	318	330	rBV	109933	162431	35.42%	4.523%
5	2.133	337	340	348	rVB10	4607	5096	1.11%	0.142%
6	3.818	854	864	886	rBV	39963	139410	30.40%	3.882%
7	4.259	988	1001	1022	rVB	86360	222136	48.44%	6.186%
8	4.963	1205	1220	1247	rBV4	176724	458538	100.00%	12.768%
9	5.542	1385	1400	1422	rBV	128106	277867	60.60%	7.737%
10	5.995	1528	1541	1563	rBV2	107585	232132	50.62%	6.464%
11	6.924	1818	1830	1846	rBV2	40842	82354	17.96%	2.293%
12	7.249	1919	1931	1946	rBV	185860	333756	72.79%	9.294%
13	7.561	2018	2028	2042	rBV3	23917	45252	9.87%	1.260%
14	8.034	2165	2175	2203	rBV	170113	380528	82.99%	10.596%
15	8.792	2401	2411	2431	rBV	199514	339224	73.98%	9.446%
16	10.162	2824	2837	2849	rBV2	81876	134132	29.25%	3.735%
17	11.136	3131	3140	3147	rVB2	3776	5351	1.17%	0.149%
18	11.194	3147	3158	3175	rBV	199567	324238	70.71%	9.029%
19	11.567	3262	3274	3289	rBV	184916	306799	66.91%	8.543%
20	12.204	3462	3472	3476	rBV10	4473	7336	1.60%	0.204%




Sum of corrected areas: 3591198

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051823\
Data File : VV031086.D
Acq On : 18 May 2023 10:31
Operator : SY/MD
Sample : VV0518WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK340

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

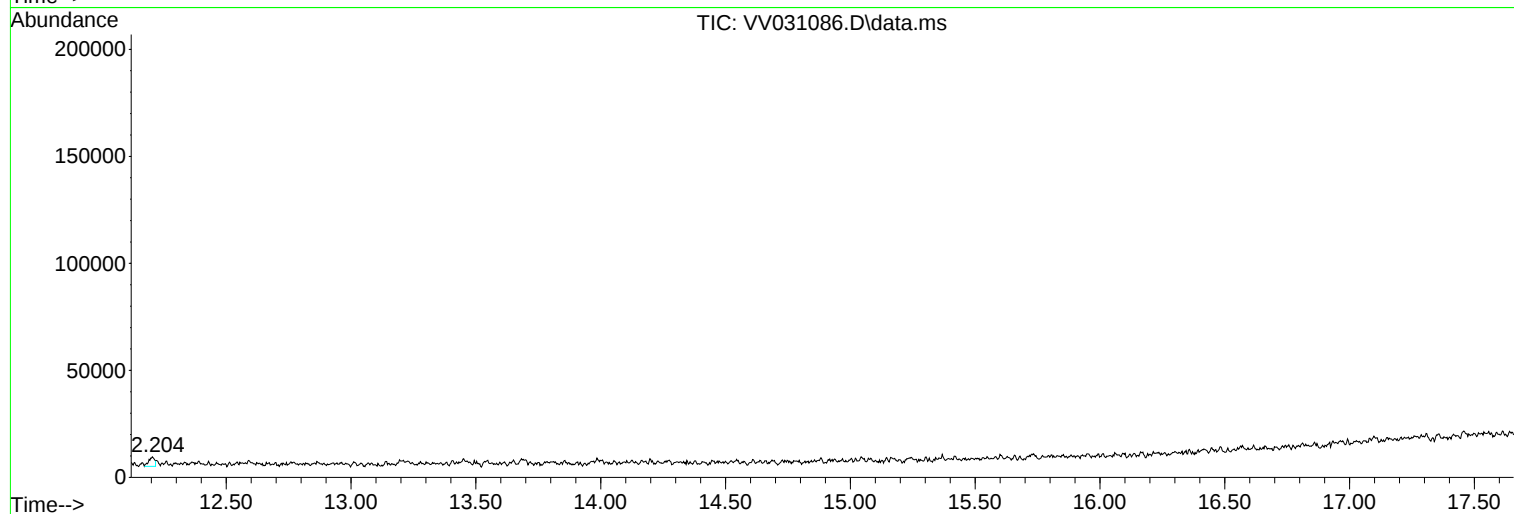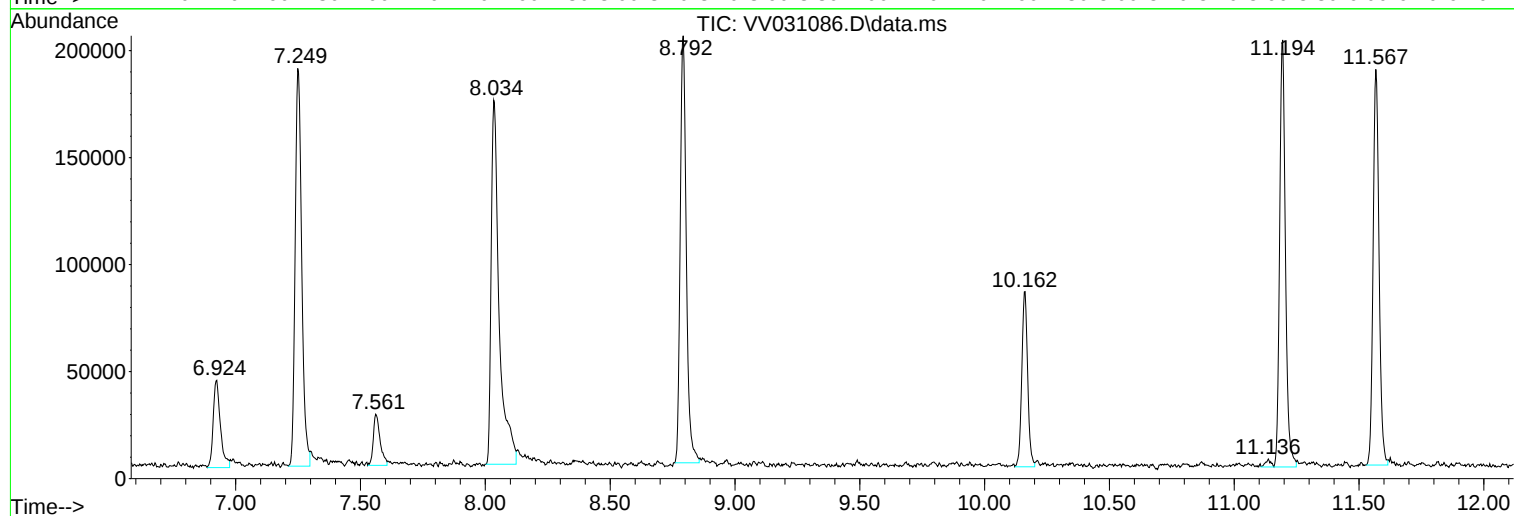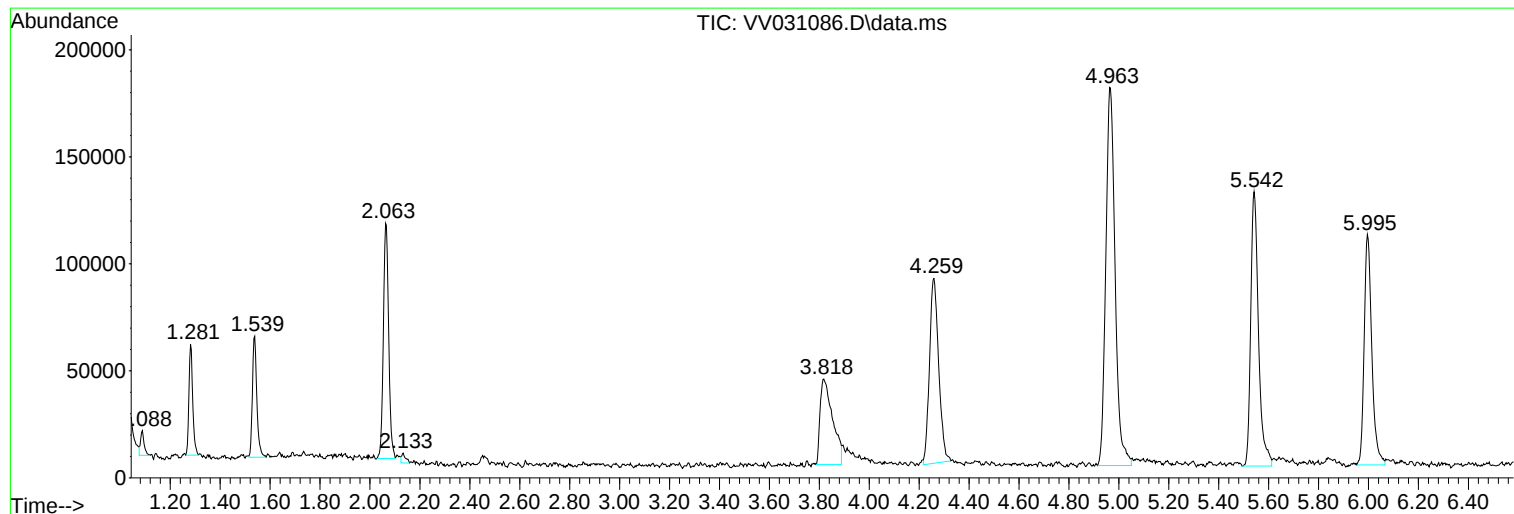

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051823\
Data File : VV031086.D
Acq On : 18 May 2023 10:31
Operator : SY/MD
Sample : VV0518WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK340

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051823\
Data File : VV031086.D
Acq On : 18 May 2023 10:31
Operator : SY/MD
Sample : VV0518WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK340

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc