

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051823\
 Data File : VV031090.D
 Acq On : 18 May 2023 14:40
 Operator : SY/MD
 Sample : 02822-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CONQ3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031090.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.089	12	15	22	rVB	11799	10506	2.56%	0.293%
2	1.285	68	76	85	rBV	38864	43415	10.57%	1.211%
3	1.539	147	155	168	rBV	48409	60006	14.61%	1.674%
4	2.066	310	319	334	rVB	88113	130773	31.84%	3.648%
5	3.822	852	865	888	rBV2	36681	135583	33.01%	3.783%
6	4.259	984	1001	1023	rBV2	79346	209803	51.08%	5.853%
7	4.966	1202	1221	1243	rBV3	157463	410732	100.00%	11.459%
8	5.542	1389	1400	1424	rBV	136940	290507	70.73%	8.105%
9	5.995	1530	1541	1560	rBV	98220	205470	50.03%	5.732%
10	6.921	1820	1829	1843	rBV	38010	73576	17.91%	2.053%
11	7.249	1920	1931	1953	rBV	159415	293955	71.57%	8.201%
12	7.561	2020	2028	2042	rBV2	21561	40604	9.89%	1.133%
13	7.882	2118	2128	2140	rVB2	19763	36042	8.78%	1.006%
14	8.037	2162	2176	2205	rBV	172733	390746	95.13%	10.901%
15	8.792	2397	2411	2428	rBV	213089	364058	88.64%	10.157%
16	10.159	2825	2836	2849	rBV	77556	126409	30.78%	3.527%
17	10.333	2880	2890	2903	rVB	54741	94405	22.98%	2.634%
18	11.194	3145	3158	3172	rBV	216281	352937	85.93%	9.846%
19	11.503	3246	3254	3255	rBV7	5507	5818	1.42%	0.162%
20	11.567	3263	3274	3289	rBV	176672	279980	68.17%	7.811%
21	12.204	3460	3472	3483	rVB3	16606	29092	7.08%	0.812%




Sum of corrected areas: 3584417

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051823\
Data File : VV031090.D
Acq On : 18 May 2023 14:40
Operator : SY/MD
Sample : 02822-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONQ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

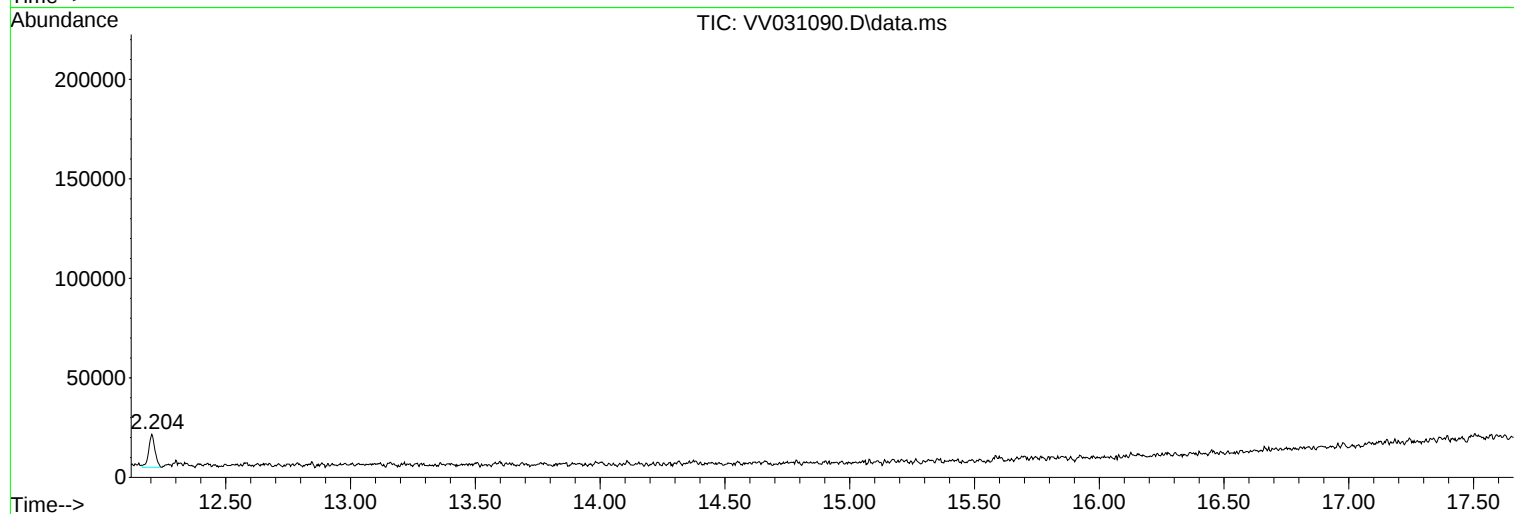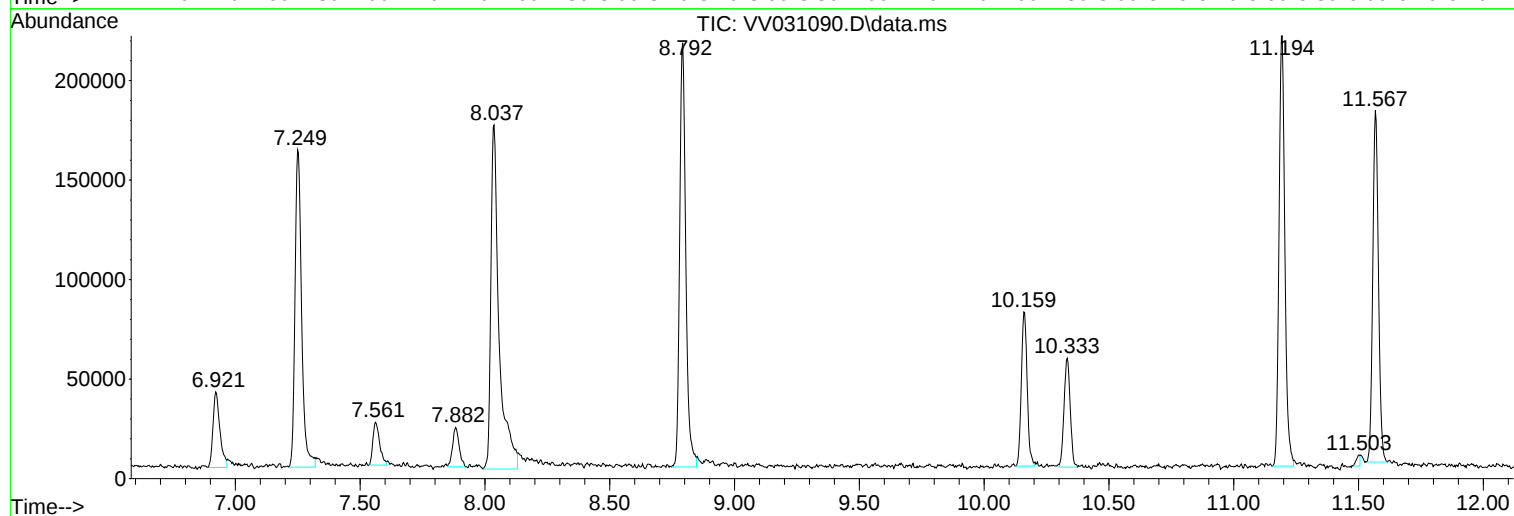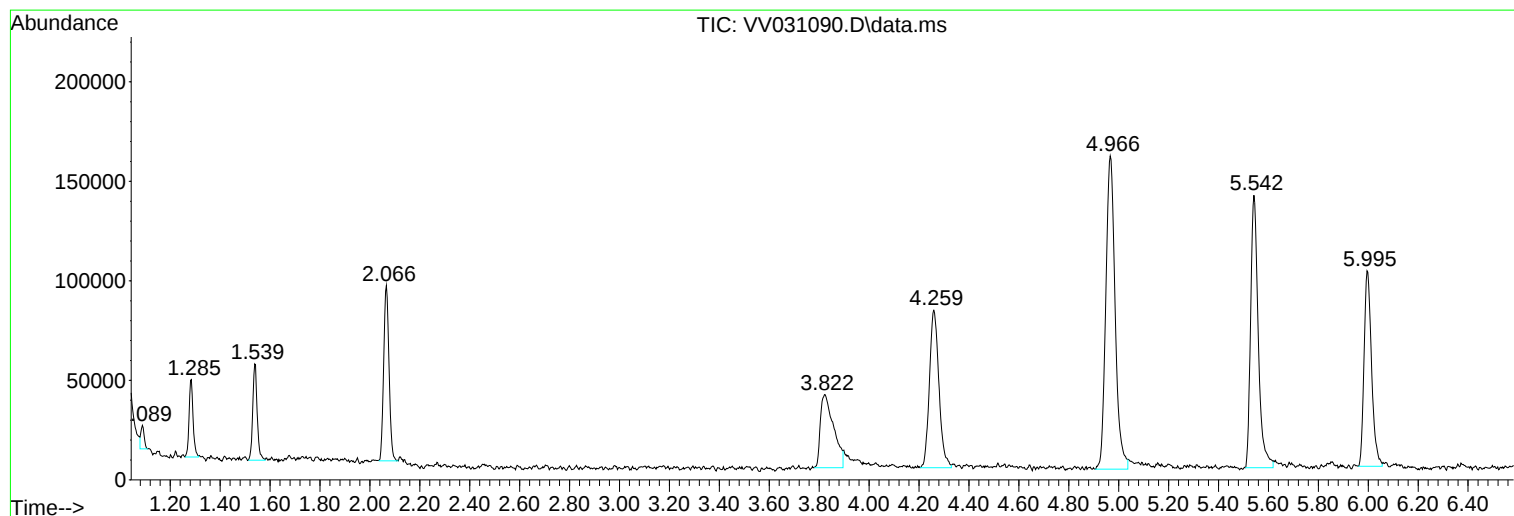

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051823\
Data File : VV031090.D
Acq On : 18 May 2023 14:40
Operator : SY/MD
Sample : 02822-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONQ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051823\
Data File : VV031090.D
Acq On : 18 May 2023 14:40
Operator : SY/MD
Sample : 02822-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONQ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc